

USER MANUAL





Intellectual property information

Fisher & Paykel Healthcare products:

F&P, Airvo, AirSpiral, Optiflow, WigglewiNG and Wigglepads are trademarks of Fisher & Paykel Healthcare Limited.

For patent information refer to: www.fphcare.com/ip

For more information, please contact your local Fisher & Paykel Healthcare representative.

Compatible third-party products:

Masimo



Masimo®, Adaptive Probe Off Detection®, APOD®, LNCS®, SET®, Signal Extraction Technology ®, Signal I.Q.®, uSpO₂®, X-Cal®, RD SET™ are trademarks of Masimo Corporation.

This device is covered under one or more of patents as set forth at: http://www.masimo.com/patents.htm

No Implied License: Possession of this device does not convey any express or implied license to use the device with unauthorized sensors or cables that would, alone, or in combination with this device, fall within the scope of one or more of the patents relating to this device.

Non-authorized Accessories: Masimo technology is designed to operate together with Masimo cables, sensors and accessories as an integrated system. When any component of the system is compromised, erroneous measurements can occur. Accordingly, the use of unauthorized sensors or accessories, such as third party reprocessed, or copycat sensors can yield unreliable results when used with a Masimo device. The performance of Masimo technology is not validated when used with any unauthorized sensor or accessory.

Masimo SET is the pulse oximetry technology proven to provide accurate measurements under the challenging monitoring conditions of low perfusion and patient motion as supported by over 100 clinical studies.

Medtronic/Nellcor

Nellcor[™] SpO₂ technology from

Medtronic

Nellcor™, OxiMax™, OxySoft™, Oxymax™, Satseconds™, Medtronic™ are trademarks of Medtronic PLC.

For patent information refer to: http://medtronic.com/patents

No Implied License: Possession or purchase of this device does not convey any express or implied license to use the device with unauthorized consumable products which would, alone, or in combination with this device, fall within the scope of one or more patents relating to this device and/or consumable products.

The Nellcor Oxicable is based on Covidien Sales' proprietary technology and should only be used with Nellcor branded sensors for proper operation and performance.

Nonin



Nonin®, Xpod®, PureLight®, PureSAT®, FlexiWraps®, Flexi-Form® are trademarks of Nonin Medical Inc.

For patent information refer to: www.nonin.com

Using any sensors other than Nonin-branded PureLight® sensors with the Nonin Xpod USB connector may result in inaccurate performance (of the Airvo™ 3 and/or Nonin products) and will void the Nonin product warranty.

Before you start

- This user manual is for instructions on using the Airvo 3.
- This user manual is intended for healthcare professionals. While the information provided is believed to be accurate, it is not a substitute for exercising professional judgement.
- Read this user manual, including all warnings, before using the Airvo 3.
- Before the Airvo 3 is used for the first time, it must be set up according to the instructions in the Airvo 3 Technical Manual.
- · Some accessories may not be available in certain countries. Please contact your local Fisher & Paykel Healthcare representative for more information.
- If any device or accessory label is damaged or unreadable, contact your Fisher & Paykel Healthcare representative for a replacement.

Additional resources

- If using the Disinfection Kit to reprocess the Airvo 3, refer to the Disinfection Kit Manual provided with the Disinfection Kit (900PT600).
- · Refer to user instructions supplied with individual accessories for correct use and additional safety information.
- · Refer to the Airvo 3 Technical Manual for initial setup, maintenance, servicing and additional troubleshooting instructions.
- · Visit the Airvo 3 website at: www.fphcare.com/airvo3 to download user instructions including this user manual.
- For assistance from your Fisher & Paykel Healthcare representative contact us at: www.fphcare.com/contact-us.

Conventions used in this manual



✓! Warning

A warning alerts the user to a potential hazard with use or misuse of the device which, if not avoided, could result in death or serious injury.



Caution

A caution alerts the user to a potential hazard with use or misuse of the device which, if not avoided, could result in minor or moderate injury.



A note emphasizes information important for using the Airvo 3 correctly.

Contents

Be	Sefore you start				
1	Intro	oduction	4		
	1.1	Intended/indications for use	4		
	1.2	Contraindications	4		
	1.3	Side-effects	4		
2	Safe	ety information	4		
	2.1	General	4		
	2.2	Supplementary oxygen			
3		erview	7		
_					
	3.1	Identifying system components.	7		
	3.2	Identifying device components	8		
	3.3	Navigating the user interface	9		
4	Pre	paring the Airvo 3	11		
	4.1	Equipment required	11		
	4.2	Airvo 3 setup	13		
	4.3	Supplementary oxygen	14		
5	Usir	ng the Airvo 3	16		
	5.1	Getting started	16		
	5.2	Optiflow high flow therapy settings			
	5.3	Starting Optiflow high flow therapy			
	5.4	During therapy			
	5.4				
		Mobility and battery operation.			
	5.6	Stopping therapy	24		
6	Mor	nitoring data	25		
	6.1	Patient data	25		
	6.2	Live value graphs	26		
	6.3	Long term graphs	26		

7	7 Troubleshooting 2					
	7.1	Alarms	. 27			
	7.2	Alarm priority	. 27			
	7.3	Auditory information signals	. 27			
	7.4	Viewing alarm details	. 28			
	7.5	Checking the alarm system.	. 28			
	7.6	Airvo 3 alarms	. 28			
8	Doni	rocessing	34			
_	кері	ocessing				
	8.1	Airvo 3 device exterior reprocessing.	. 34			
	8.2	Outlet elbow reprocessing	. 35			
	8.3	Schedule for changing accessories	. 37			
	8.4	Replacing the air filter	. 37			
	8.5	Servicing	. 37			
9	Puls	e oximetry	38			
	9.1	Pulse oximetry warnings, cautions, and notes	38			
	9.2	Setup for pulse oximetry				
	9.3	During therapy				
		5 ,,5				
	9.4	Description of measurements				
	9.5	Description of settings and alarms				
	9.6	Alarm and measurement settings				
	9.7	Troubleshooting	. 45			
Sp	ecific	rations	47			
Gle	Glossary 52					
Ap	pend	lix 1. Patient consumables	53			
Αp	Appendix 2. Parts and accessories 54					
Ap	pend	lix 3. Pulse oximetry accessories	55			
Ap	pend	lix 4. Humidification behavior during battery operation	59			

1. Introduction

The Airvo 3 is designed to deliver Optiflow™ high flow therapy to spontaneously breathing patients.

A blower inside the Airvo 3 entrains flows of room air of 2 - 70 L/min, which may be blended with oxygen from high-pressure sources (such as wall supplies or bottles) or low-pressure sources (such as flowmeters). The air-oxygen mixture is then warmed and humidified in the water chamber, before being transported through the heated breathing tube to a nasal, tracheostomy or mask patient interface.

The Airvo 3 is powered by wall power supply, with internal battery backup to provide continuity of therapy during intra-hospital transport.

Intended use/indications for use 1.1

The Airvo 3 is for the treatment of spontaneously breathing patients who would benefit from receiving high flow warmed and humidified respiratory gases. This includes patients who have had upper airways bypassed. The flow may be from 2 - 70 L/min depending on the patient interface. The Airvo 3 is for patients in hospitals and subacute facilities.

The Airvo 3 can deliver these high flow gases through nasal cannula to augment the breathing of spontaneously breathing neonate, infant, child, adolescent and adult patients suffering from respiratory distress and/or hypoxemia in the hospital setting. The Airvo 3 is not intended to provide total ventilatory requirements of the patient and is not for use during field transport.

1.2 **Contraindications**

Contraindications are therapy-specific. Refer to instructions of patient interfaces and/or tube and chamber kits for therapy-specific contraindications.

Side-effects 1.3

Side-effects are therapy-specific. Refer to instructions of patient interfaces and/or tube and chamber kits for therapy-specific side-effects.

2. Safety information

The Airvo 3 and accessories are to be operated by, or under the supervision of, qualified personnel only. Read this manual, particularly all warnings, cautions and notes, and the instructions for use supplied with all accessories before using the Airvo 3.

2.1 General



∕!\ Warnings

- The Airvo 3 is not intended for life support. Do not use Airvo 3 on patients who cannot tolerate a brief interruption of therapy.
- Appropriate patient monitoring is required for all patients using the Airvo 3.
- Delivery of respiratory gases may generate positive airway pressure. This must be considered where positive airway pressure could have adverse effects on a patient. To avoid serious injury, appropriately monitor the patient for risk factors of airway and lung pressure iniury.
- Anybody connecting patient consumables, accessories or spare parts to the Airvo 3 is accountable for the compatibility of the device and those patient consumables, accessories and/or spare parts.
- Do not use any patient consumables, accessories or spare parts that are not listed in this user manual, or the Airvo 3 Technical Manual. Incompatible consumables, parts or accessories could affect the quality of therapy, injure the patient, decrease electromagnetic immunity or increase electromagnetic emissions.
- · Use only patient interfaces, heated breathing tubes, water chambers and filters specified in this manual to prevent disconnection during use, especially when moving the Airvo 3.
- Do not use antistatic or electrically conductive patient breathing circuits with the Airvo 3.
- · Do not connect the Airvo 3 to the battery of a battery-powered wheelchair, which may compromise device performance and therapy delivered.
- Do not start or operate the Airvo 3 unless the device setup, including all accessories, is verified to be correct.
- Carefully route accessories, cords and cables, including the breathing tube, to reduce the possibility of patient entanglement or strangulation.
- Visually inspect the Airvo 3 and accessories before use and replace if damaged or suspected to be damaged. Using a damaged device or accessories may impair performance and/or compromise safety.
- Make sure the auditory alarm signal is audible to the operator who will respond to alarms by following the instructions in section 7.5 to test the alarm before starting therapy.
- Do not use an Airvo 3 on more than one patient at any one time.
- · Do not use accessories beyond the maximum period of use specified in this manual. Exceeding the maximum use period can result in serious injury, including infection.

- Do not expose the Airvo 3 battery to water, fire or excessive heat. Do not crush, disassemble or puncture the battery, or short-circuit the connector terminals.
- Do not use the Airvo 3 as an apnea monitor.
- Do not use the Airvo 3 for arrhythmia analysis.
- In the event of a battery leaking, do not allow the liquid to come in contact with the skin or eyes. If contact has been made, wash the affected area with copious amounts of water and seek medical advice.
- Seek medical advice immediately if a cell or a battery has been swallowed.
- · Changes or modifications not expressly approved by Fisher & Paykel Healthcare voids the user's authority to operate the device.
- The therapy delivered to the patient can be impacted by the use of a pneumatic/iet nebuliser. Refer to compatible accessories and drug manufacturer instructions for correct usage.
- Do not use any solutions, suspensions, emulsions, anesthetic or respirable gases that are not identified in these user instructions. They may not be compatible with the patient consumables, device or accessories.
- Use only genuine F&P replacement battery modules to prevent damage to the Airvo 3, excessive temperatures, fire or explosion.

Operating environment

- Do not use the Airyo 3 at an altitude or temperature outside the rated range listed in the specifications section of the manual. Using outside of these ranges can compromise the equipment performance which consequently can result in degradation of the health of the
- Do not use the Airvo 3 when outside the operating conditions listed in the specifications section. Therapy may be compromised outside this range.
- Do not use the Airvo 3 in a magnetic resonance imaging (MRI) environment.
- Do not use the Airvo 3 with, or in the presence of, a flammable anesthetic mixture with air or oxygen.
- Do not use the Airvo 3, or accessories, during defibrillation.
- Do not use the Airvo 3, or accessories, near any ignition source, including electrosurgery, electrocautery, or laser surgery instruments. Exposure to oxygen increases the risk of fire that may result in patient injury.
- Do not use the Airvo 3. or accessories during electrocautery.
- Explosion hazard: Do not use the Airvo 3 in the presence of flammable anesthetics or other flammable substances in combination with air, oxygen-enriched environments, or nitrous oxide.
- Do not use the Airvo 3 in a hyperbaric chamber.
- · Avoid using the Airvo 3, or accessories, adjacent to, or stacked with, other equipment, which could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.
- The Airvo 3 is not designed for use in the home.

/! \ Caution

• The emissions characteristics of this equipment make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required) this equipment might not offer adequate protection to radio-frequency communication services. The user might need to take mitigation measures, such as relocating or re-orienting the equipment.

To avoid burns

- Do not touch the hot surface of the heater-plate or chamber base.
- Never operate the Airvo 3 if:
 - the heated breathing tube has been damaged in any way including holes, tears or kinks,
 - it is not working properly, or
 - water has entered the device.
- Do not restrict ventilation around the Airvo 3, which may cause it to overheat.
- Do not block the flow of air through the Airvo 3 or breathing tube.

To avoid electric shock

- Do not store or use the Airvo 3 where it can fall, or be pulled, into water. Disconnect the power cord and stop using the Airvo 3 if water has entered the case.
- To protect from electric shock, always remove the sensor and completely disconnect the pulse oximeter before bathing the patient.
- Never operate the Airvo 3 if it has, or is suspected of having:
 - been dropped or damaged,
 - a damaged power cord or plug, or
 - been dropped into water.
- See the Airvo 3 Technical Manual for instructions to replace a damaged power cord.
- Do not attempt to adjust, repair, open, disassemble or modify the Airvo 3, pulse oximeter equipment, or accessories except as described in this user manual or the Airvo 3 Technical Manual. Return the Airvo 3 to your Fisher & Paykel Healthcare representative for servicing, if necessary.
- Do not touch the patient at the same time as any conductive parts of the device, such as USB ports.



(!) Notes

• If a serious incident has occurred while using this device please inform your local Fisher & Paykel Healthcare representative and Competent Authority in your country.

2.2 Supplementary oxygen




⚠ Warnings

- You must take special care when using supplementary oxygen to reduce the risk of fire. Keep all sources of ignition away from the Airvo 3 and, preferably, not in the same room as the Airvo 3 during use.
- Do not use supplementary oxygen while smoking, near sparks or open flames.
- · A spontaneous and violent ignition may occur if oil, grease or greasy substances contact oxygen under pressure. Keep these substances away from all oxygen equipment.
- The Airvo 3 is a high flow device. Ensure the oxygen supply is designed to provide enough oxygen flow for all connected equipment, particularly when the supply is shared by multiple devices.
- · Only connect pure oxygen to the oxygen inlet ports on the Airvo 3. The oxygen concentration displayed will be wrong if any other gas, or mixtures of gases, is connected.
- Only use lotions and/or salves that are labeled as oxygen-compatible to avoid the risk of fire and burns.


This section shows the Airvo 3 system and compatible accessories.


3.1 Identifying system components

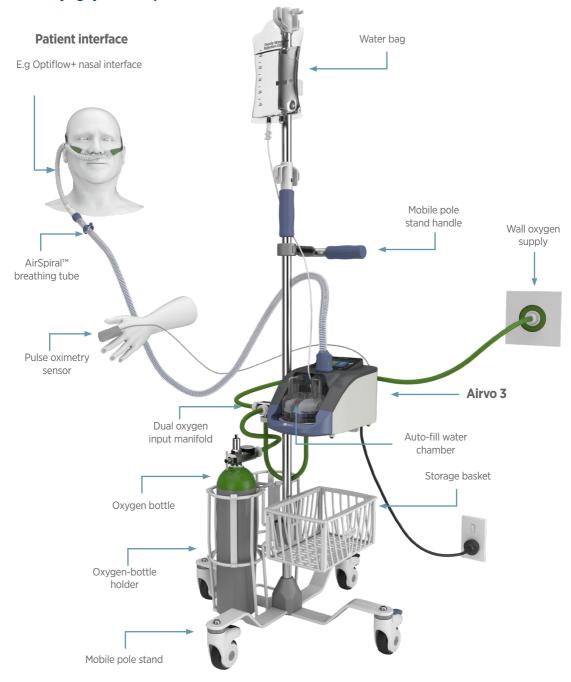


The Airvo 3 System

3.2 Identifying device components

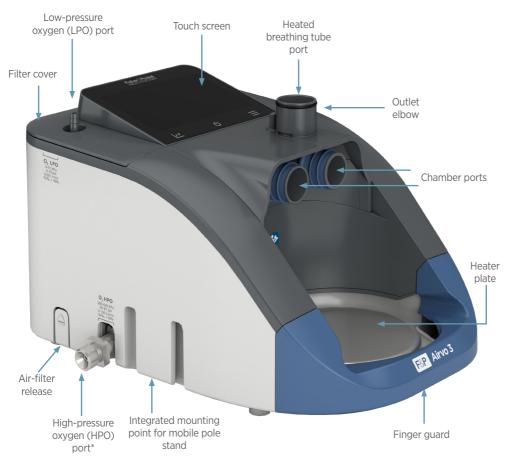

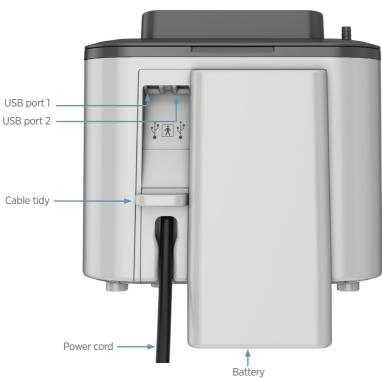

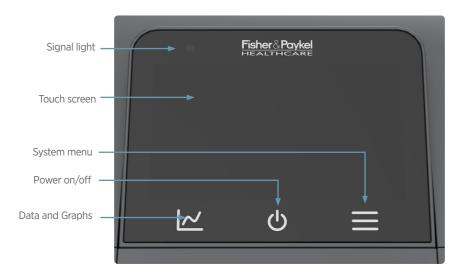

3.3 Navigating the user interface

The Airvo 3 touch screen provides access to therapy and device status, settings and alarms. You interact with the user interface by:

- touching elements on the screen to open setting screens, make selections and change values, and
- swiping up/down to scroll through menus that are only partly displayed.

3.3.1 Home screen





To ensure responsiveness keep Airvo 3 touchscreen clean and dry. Performance may be reduced if the screen is allowed to become wet.

3.3.2 Message bar

The Message bar shows the current state of therapy delivery, confirms settings changes and displays alarms. Example messages are shown in the table below.

Message bar	Description
Standby - No therapy being delivered \Box \Box \Box	Breathing gases are not being delivered to the patient. Tap the Start button to begin therapy.
Therapy on ♥ 🗓 1000 🗮	Breathing gases are being delivered. Tap the Stop button, then confirm action to return to standby mode.
△ Leak Detected ば め =	Active alarms are displayed on top of other messages. Tap the alarm for details or press 💢 to temporarily pause the alarm audio. See section 7 for troubleshooting alarms.

3.3.3 Status indicators

The following icons may be displayed in the Message bar.

Icon	Description
	Audio pause
Ϋ́	The Airvo 3 is being powered from the wall power supply
100%	Status of the internal battery
50%	50% of the battery charge is remaining
50%	Battery is charging and 50% of the charge is remaining
50%	Battery is not charging properly
lacktriangle	Battery is missing or faulty
	Battery is due for replacement
Ð	Touch display is locked to prevent accidental changes
ψ	An Airvo 3 USB storage device is connected to one of the USB ports

^{*}Check the battery is properly installed. Replace the battery if the problem persists.


3.3.4 Signal light

The signal light flashes when any alarm is active. Its color indicates the highest priority alarm that is active. See section 7 for troubleshooting alarms.



3.3.5 System menu

The system menu provides access to additional settings and information. Tap \equiv to open the system menu when the Home screen is displayed.



Menu item	Description
Pulse Oximeter Alarms and Settings	Configure the pulse oximetry settings including $\ensuremath{SpO_2}$ alarms
Lock Screen	The lock screen can prevent accidental settings changes
Device Info	Displays the version, disinfection, and battery information
System Settings	Change advanced Airvo 3 settings, limits and behaviors. Refer to the Airvo 3 Technical Manual for more information

3.3.6 Data and Graphs screen

The Data and Graphs screen displays current and previous measurements and settings for the current patient.

Tap 🗠 to open the Data and Graphs screen when the Home screen is displayed. The values available depends on the active therapy mode

4. Preparing the Airvo 3

Review the safety information in section 2 before proceeding. Refer to appendices 1 - 3 for a list of consumables and accessories that have been validated for use with the Airvo 3.

4.1 **Equipment required**

You will need:

- Airvo 3 attached to a mobile pole stand,
- · clean and disinfected outlet elbow.
- bag of USP sterile/distilled water for inhalation (or equivalent).

Outlet elbows can be processed in two different ways:

Disinfection kit (900PT600)

For hospitals using the disinfection kit for reprocessing: A clean and disinfected outlet elbow will already be installed in the Airvo 3. Remove the clean storage cover and/or the red disinfection tube before use.

Washer-disinfector

For hospitals using a washer-disinfector for reprocessing: obtain a clean and disinfected outlet elbow, e.g. from your Central Sterile Services Department (CSSD) system.

If supplementary oxygen is prescribed for your patient, you will need either:

- · high-pressure oxygen hoses to connect the Airvo 3 to the wall oxygen supply or an oxygen-bottle regulator, or
- low-pressure oxygen tubing to connect the Airvo 3 to a flowmeter.



Warnings

Only use patient consumables and accessories that are compatible with the Airvo 3 (see Appendix 1-3). Do not modify patient consumables or accessories in any way.

4.1.1 **Optiflow high flow therapy**

To provide Optiflow high flow therapy, you will need a:

- 1. Breathing tube and chamber kit.
- 2. Optiflow patient interface.

Refer to Appendix 1 for a list of compatible consumables.

Nasal interface



Optiflow+ Optiflow 3S Optiflow+ Duet




Optiflow Junior 2 Optiflow Junior 2+

Tracheostomy interface



Optiflow+ tracheostomy interface

Mask interface adapter



Optiflow+ mask interface adapter

4.2 Airvo 3 setup

Standard aseptic techniques should be followed to minimize contamination when handling the Airvo 3 and accessories.



1. Check Airvo 3 height

Check that the Airvo 3 is attached securely to the mobile pole stand and is below the patient's head height.

Position the Airvo 3 so that the power cord connection to the wall power supply is easily accessible and can be disconnected if necessary.



∠!\ Caution

Do not place the Airvo 3 where controls can be changed by the patient.



2. Connect the outlet elbow (if applicable)

This step applies if your hospital uses a washer-disinfector to clean and disinfect the outlet elbow. This step does not apply if your hospital uses the disinfection kit (900PT600).

Insert the clean, disinfected outlet elbow into the slot on the top of the Airvo 3.



∠! Warning

Make sure the Airvo 3 is off when connecting the outlet elbow.




3. Assemble the water chamber

Open the tube and chamber kit and remove the MR290 auto-fill water chamber and chamber adapter.

Remove the blue port caps from the chamber by pulling the tear tab upwards then remove the bracket holding the water supply tube.

Fit the supplied adapter over the two vertical ports on the chamber and push on fully then clip the water supply tube into position.



4. Insert the water chamber

Fit the water chamber to the Airvo 3, sliding the chamber past the finger guard onto the heater-plate. Take care to align the port adapter with the blue ports on

Ensure the water chamber is fully inserted by pushing firmly on the front of the chamber until it slides past the finger guard.

To remove the water chamber, grip the port adapter and pull the chamber away from the Airvo 3.



✓!\ Warnings

To avoid burns:

Do not start therapy without the water chamber in place.

Do not touch the heater-plate, water chamber or chamber base during

Exercise caution when removing the chamber.

To avoid electrical shock:

When handling the Airvo 3 with the water chamber in place, avoid tilting the device to prevent any chance of water entering the unit enclosure.

Do not use the MR290 auto-fill water chamber if it has been dropped, allowed to run dry or damaged in any way. This could lead to the chamber overfilling.




5. Connect the water bag

Attach the sterile water bag to the hanging bracket 50 cm above the Airvo 3. Remove the spike from the chamber bracket and push the bag spike into the fitting at the bottom of the bag.

Open the vent cap on the side of the bag spike.



Only use USP sterile/distilled water, suitable for inhalation, to fill the water chamber. Adding other substances can adversely affect the humidifier and therapy delivered.



6. Check the water level


Check that water flows into the chamber and remains below the maximum

The chamber will automatically maintain the correct water level until the water bag is empty.



∕!\ Caution

Do not use the MR290 auto-fill chamber if the water level rises above the maximum water-level line. This may lead to water entering the patient's airway.



7. Install the breathing tube

Connect the breathing tube by lining up the pins on top of the Airvo 3, pushing down until you hear a click and the tube locks into place.

To remove the breathing tube, squeeze the sides of the connector and pull up.




Warnings

Do not use an insulating sleeve or any similar accessories which are not recommended by Fisher & Paykel Healthcare.



Make sure the outlet elbow is installed in the Airvo 3 before attaching the heated breathing tube.

See step 2 "Connect the outlet elbow (if applicable)" above.




Supplementary oxygen

The Airvo 3 provides two options for connecting supplementary oxygen:

- A high-pressure oxygen (HPO) inlet port, and
- A low-pressure oxygen (LPO) inlet port.

The high-pressure oxygen inlet port is connected to the wall oxygen supply or to the pressure regulator on an oxygen bottle. The ability of the Airvo 3 to provide the target FiO₂ is limited by the line pressure of the high-pressure inlet port (HPO). If the Airvo 3 is unable to maintain the target FiO₂, the device will generate a "FiO₂ Below Target" alarm. The low-pressure oxygen inlet port is connected to an external flowmeter, typically a rotameter.





∠!\ Warnings

You must take special care when using supplementary oxygen to reduce the risk of fire. Keep all sources of ignition away from the Airvo 3 and, preferably, not in the same room as the Airvo 3 during use.

Do not use supplementary oxygen while smoking, near sparks or open flames.

When using bottled oxygen, ensure the volume remaining in the bottle is sufficient for the therapy planned.

Connect only pure oxygen gas to the oxygen inlet ports on the Airvo 3. The oxygen concentration displayed will be wrong if any other gas, or mixtures of gases, is connected.

The oxygen concentration delivered to the patient can be affected by changes to the oxygen setting, patient interface or obstructions in the air path.

Only use lotions and/or salves that are labeled as oxygen-compatible to avoid the risk of fire and burns.

Appropriate patient monitoring must be used at all times.

Make sure that all oxygen connectors are tightened sufficiently to prevent leaks.

As the low-pressure oxygen (LPO) inlet port uses an alternative small-bore connector design different from those specified in the ISO 80369 series, there is a possibility that a misconnection can occur with a medical device using a different alternative small-bore connector, which can result in a hazardous situation causing harm to the patient. Special measures need be taken by the user to mitigate these reasonably foreseeable risks.

During Optiflow high flow therapy, the fraction of oxygen inspired by the patient will be lower than the value displayed on the FiO₂ tile if the patient's peak inspiratory demand exceeds the flow delivered.

The Airvo 3 is a high-flow device and should only be connected to a pipeline installation designed using a diversity factor that allows for the indicated high-flow at a specified number of terminal outlets, in order to avoid exceeding the pipeline design flow, thereby minimizing the risk that the humidifier interferes with the operation of adjacent equipment.

There is a risk of fire associated with oxygen enrichment during oxygen therapy. Do not use the equipment or accessories near sparks or open flames.

Smoking during oxygen therapy is dangerous and is likely to result in facial burns or death. Do not allow smoking or open flames within the same room as the equipment or any oxygen-carrying accessories. If the patient intends to smoke, always turn the equipment off, remove the cannula and leave the room where the equipment is located. If unable to leave the room, wait 10 minutes after the equipment has been turned off.

Do not lubricate fittings, connections, tubing, or other accessories of the equipment to avoid the risk of fire and burns.

Oxygen makes it easier for a fire to start and spread. Do not leave the nasal cannula or mask on bed coverings or chair cushions, if the device is turned on, but not in use; the oxygen will make the materials more flammable. Turn the device off when not in use to prevent oxygen enrichment.

It is the responsibility of the responsible organization to ensure that the oxygen source is compatible with the rated range of pressure, flowrate and oxygen concentration as marked on the equipment and indicated in the instructions for use as this can affect the performance of the equipment or pipeline system that can consequently result in serious deterioration of health.

Open flames during Optiflow high flow therapy are dangerous and are likely to result in fire or death. Do not allow open flames within 2 m of the equipment or any oxygen-carrying accessories.




Do not connect an oxygen supply to both the high-pressure oxygen inlet port and the low-pressure oxygen inlet port at the same time. Using the low-pressure inlet at the same time as the high-pressure inlet may cause incorrect oxygen delivery and a FiO₂ Above Target alarm.



The built-in oxygen analyzer uses ultrasonic measurement technology. It does not require in-field calibration.

4.3.1 High-pressure oxygen (HPO) source

When oxygen is connected to the HPO port, the Airvo 3 directly controls the oxygen input to meet the target FiO₂ setting.




4.3.2 Low-pressure oxygen (LPO) inlet port

When using the LPO port, the amount of oxygen taken in by the Airvo 3 is controlled by an external flowmeter. Connect a tube from the external flowmeter to the LPO port. Make sure that the flowmeter is turned off whenever the Airvo 3 is not delivering therapy.

When using the low-pressure oxygen inlet port, monitor the oxygen concentration displayed on the Home screen. The oxygen flow-regulator must be adjusted manually to maintain the prescribed oxygen concentration when changing the respiratory gas flow rate.

Clinicians may configure a High FiO₂ alarm to discourage use of high FiO₂ values in particular clinical environments.

The High FiO₂ alarm can be disabled or a threshold between 30% and 95% can be selected when the Airvo 3 is initially set up for your environment (see Oxygen high alarm threshold, Airvo 3 Technical Manual). The alarm threshold is displayed on the Titrate FiO₂ screen, if enabled. Tap the FiO₂ tile to open the Titrate FiO₂ screen.






Turn off the low-pressure oxygen source whenever the Airvo 3 is not delivering therapy, to ensure that oxygen does not build up inside the device.

5. Using the Airvo 3

5.1 **Getting started**



Turn on the Airvo 3

Plug the Airvo 3 power cord into the wall power supply.

Lock the wheels of the mobile pole stand to prevent the Airvo 3 from

Turn on the Airvo 3 by holding down the Power on/off button for 2 seconds.



∕!\ Warning

Make sure the Airvo 3 is dry before plugging the power cord into the wall power supply to avoid a potential electric shock.

Do not cover or position next to materials that can block the gas intake, thereby interfering with the patient therapy.



If the Airvo 3 has been unused and disconnected from the wall power supply for some time, the device will not power on without being plugged in.



✓!\ Warnings

The Airvo 3 must be cleaned and disinfected between patients. Refer to section 8 for the steps required to reprocess the Airvo 3 between patients.

Do not exceed the maximum use period for single-patient-use accessories and consumables (see section 8.3 for the schedule for changing accessories).





Review disinfection state

The Airvo 3 will ask you if it will be used on: the same patient who last used the device (tap Same Patient)

OR

a new patient (tap New Patient).

For a new patient, check that:

- 1. The outlet elbow has been cleaned and disinfected.
- 2. A new tube and chamber have been installed.



Review disinfection state (if the disinfection method is set to disinfection kit only)

For a new patient, check that:

1. The outlet elbow has been cleaned and disinfected.

The Airvo 3 will indicate the outcome of the last disinfection cycle:



Green: The previous disinfection cycle was completed successfully.



Orange: A successful disinfection cycle has not been performed. Please run a successful disinfection cycle before use on a new patient.



Red: The previous disinfection cycle failed to complete. Please run a successful disinfection cycle before use on a patient.

The number of successful disinfection cycles completed by the Airvo 3 is displayed in the lower left hand corner under 'Disinfection count'.

2. A new tube and chamber have been installed.


5.2 Optiflow high flow therapy settings

The default range of Optiflow high flow therapy settings is shown below. Some settings may have been limited, or disabled, when the device was initially set up for its intended clinical environment. Refer to the Airvo 3 Technical Manual for details.

Settings are persistent and will retain their previous value when the Airvo 3 is turned on. Selecting New Patient when reviewing the disinfection state (see section 5.1 above) applies the default values for its intended clinical environment to all settings.

Setting	Range	Description
Target humidity	31 - 37 °C	Target humidity for the respiratory gas supplied to the patient
Target flow	2 - 70 L/min	Flow rate of the respiratory gas supplied to the patient
FiO ₂	21 - 100%	Target oxygen concentration for the breathing gases when an external oxygen supply is connected to the high-pressure oxygen inlet port
Expiratory relief (Target flow tile)	Off, 10%, 20%, 30%	This setting is disabled by default, and only available when the set flow is greater than 25L/min refer to the Airvo 3 Technical Manual for details. Expiratory relief automatically reduces the respiratory gas flow rate during exhalation and returns it to normal during inhalation. Indicative flow rates are displayed on the settings screen. These may differ depending on the method and strength of the patients breath

Tiles on the Home screen show current Optiflow high flow therapy settings and measurements. Only tiles relevant to connected accessories are shown.

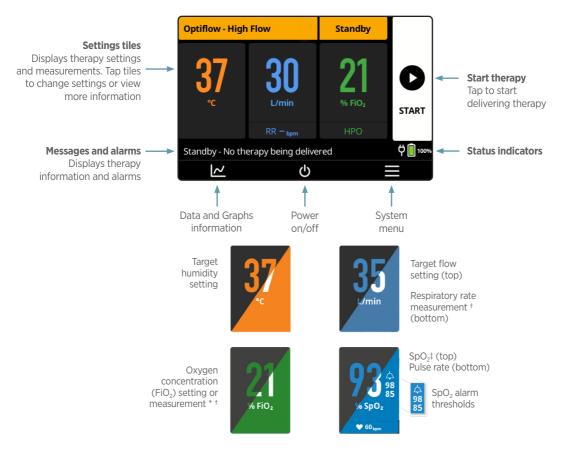

^{*} The FiO2 tile shows the breathing gas oxygen concentration setting when supplementary oxygen is connected to the high-pressure oxygen (HPO) inlet port and measured oxygen concentration when connected to the low-pressure oxygen (LPO) inlet port. Measured oxygen concentration is not available in standby mode.

 $^{^{\}dagger}$ "--" is displayed when a value is not available; values are gray when signal quality is poor.

[‡] The SpO₂ tile is displayed automatically when a compatible pulse oximeter is connected.

Starting Optiflow high flow therapy

Follow the steps below to start delivering Optiflow high flow therapy. Some settings may have been limited, or disabled, when the device was initially set up for your clinical environment. Refer to the Airvo 3 Technical Manual for details.



Adjust target humidity

- 1. Tap the target humidity tile to open the Target Humidity screen.
- 2. Use the + / buttons or slider to select a desired target humidity.
- 3. Tap Confirm to apply the change and return to the Home screen. Tap Cancel to discard any changes.



∠!\ Warnings

Airvo 3 is classified as a Category 1 humidifier for patients with bypassed airways (tracheostomies) in the following modes only: 37 °C and 10-60 L/min. Do not use any other mode for patients with bypassed airways (tracheostomies).



Patients using face masks may find high temperatures uncomfortable. Consider a target temperature of 31 °C.





Adjust target flow

- 1. Tap the target flow tile to open the Target Flow screen.
- 2. Use the + / buttons or slider to select the desired flow.
- 3. Tap Confirm to apply the change and return to the Home screen. Tap Cancel to discard any changes.

An appropriate flow rate for your patient should be prescribed following hospital protocols.



Refer to the patient interface user instructions for details.





Start therapy

Check that the breathing tube is assembled correctly and all connections are secure. Check the alarms are operating properly according to the instructions in section 7.5.

Tap the START button to begin therapy. After warming up, the Airvo 3 will play a short melody and display the message "Therapy on".



Adjust supplementary oxygen (optional)



∠! Warning

Use continuous SpO₂ monitoring on patients who would desaturate significantly if their oxygen supply is disrupted.

The FiO₂ control limits should be prescribed based on patient condition, hospital policies and clinical judgement for Optiflow nasal high flow therapy.

Oxygen connected to the high-pressure inlet port (HPO)

- 1. Tap the FiO₂ tile to open the Titrate FiO₂ screen.
- 2. Use the + / buttons or slider to select the desired FiO₂.
- 3. Tap Confirm to apply the change and return to the Home screen. Tap Cancel to discard any changes.

The Airvo 3 will automatically adjust oxygen flow to maintain the selected FiO₂.

Oxygen connected to the low-pressure inlet port (LPO)

The Airvo 3 does not directly control FiO₂. Use an external flowmeter to adjust FiO₂ to the prescribed level. The oxygen tile displays measured FiO2.




It may take a few minutes for the oxygen measurement to stabilize. The external flowmeter will need to be readjusted following changes to Airvo 3 target flow.

High FiO₂ alarm

Clinicians may configure a High FiO₂ alarm to discourage the use of high FiO₂ values in particular clinical environments. See the Airvo 3 Technical Manual for setup details.

If the alarm is enabled, the alarm threshold is displayed on the Target FiO₂

The following table shows the target flow settings able to be used with these interfaces

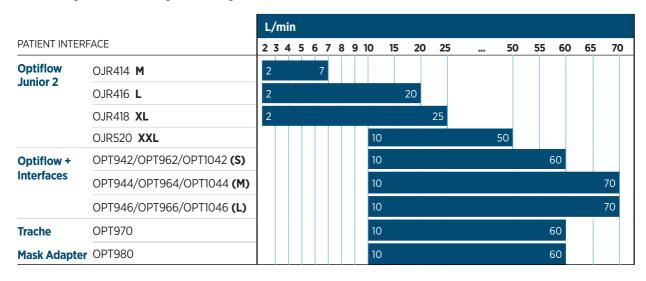



Fit the patient interface

Fit the patient interface to your patient following the user instructions supplied with the interface. Take care to follow all warnings and cautions.



Connect to the patient interface

Connect the patient interface to the connector at the end of the breathing tube.

The patient may be connected to the heated breathing tube immediately. When therapy initiation is not urgent, it is recommended to wait until the Airvo 3 plays a short melody and displays "Therapy On" in the Message bar.


Attach the breathing tube clip to the patient's clothing.



🔼 Warnings

Do not allow the breathing tube to remain in direct contact with the patient's skin for long periods of time to avoid the risk of burns. The healthcare professional shall assess the conditions for safe contact, such as duration and skin condition.

Do not cover or add heat above ambient levels to any part of the breathing tube or interface e.g. by covering with a blanket or by heating with infrared radiation, an overhead heater, or an incubator, as this can affect the quality of the therapy or injure the patient.



Do not use sealed patient interfaces with Optiflow high flow therapy, to avoid the risk of suffocation or barotrauama.

Ensure a sufficient intended leakage between the breathing system and the patient to allow the patient to exhale.



✓!\ Caution

Keep the heated breathing tube away from electrical monitoring leads (e.g. EEG, ECG/EKG, EMG, pulse oximeter) to reduce the risk of interference with the signal monitored.



(!) Note

The air may feel warm when your patient starts using the Airvo 3. This is normal. The patient should continue to breathe normally.

During therapy

Monitor the patient following hospital protocols and clinical judgement. Ensure you can hear and respond to any device alarms.


If there is an interruption to the power supply, and the battery is depleted, the Airvo 3 will raise a Power Out alarm, turn off, and not deliver any therapy to the patient. The power out alarm will sound once every 10 seconds for a minimum of 120 seconds, and the signal light above the touch screen will flash. Once power is restored the Airvo 3 can be restarted and will retain the previous therapy and alarm settinas.



If using the battery as the power source, periodically check the battery status to ensure the battery does not become depleted while therapy is being delivered.

5.4.1 Lock Screen (optional)

The lock screen can prevent accidental settings changes.

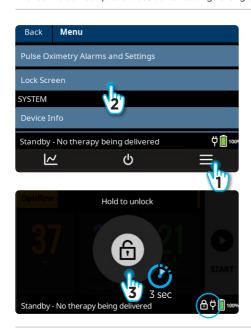

To enable the lock screen:

- 1. Tap ≡ to open the system menu.
- 2. Select Lock screen from the system menu. The symbol 🗖 is shown in the Message bar.

To disable the lock screen:

3. Touch the screen while it is locked, then hold the Unlock icon for three seconds.

5.4.2 Monitor and adjust settings

Adjust settings as needed. Most changes take effect after pressing the confirmation button but it may take a few minutes for some settings, such as target humidity, to respond to changes. Tiles show an animated ellipsis symbol (...) to indicate that a therapy setting has not yet reached its target.



5.4.3 Manage condensation

Drain excess condensate from the breathing tube by:

- 1. Disconnecting the breathing tube from the patient interface, and
- 2. Lifting the patient end of the tube so the condensate runs into the water chamber.

Reduce the flow rate below 30 L/min if the condensate does not run freely into the water chamber. Return the flow rate to the prescribed setting after draining the breathing tube.

Direct cold air away from the heated breathing tube where possible. Air conditioners, fans, open windows and other sources of cold air may increase condensation.


Consider reducing the target humidity if condensation persists.

Mobility and battery operation

The HPO (High Pressure Oxygen) dual-input manifold and internal rechargeable battery provide continuity during intra-hospital transport. Reduced humidity will be delivered when the Airvo 3 is being powered only by the battery: for more details see Appendix 4. The HPO dual-input manifold uses the oxygen supply with the highest pressure.

When transporting the Airvo 3 with your patient:

- Adjust therapy settings as necessary for intra-hospital transport.
- 2. If using supplementary oxygen:
 - · Check that the oxygen bottle contains enough oxygen for your journey.
 - Turn on the oxygen-bottle pressure regulator.
 - Disconnect the oxygen hose from the wall supply. Either attach it to a second oxygen bottle for longer trips or hook it over the Airvo mobile pole stand if additional oxygen is not required.

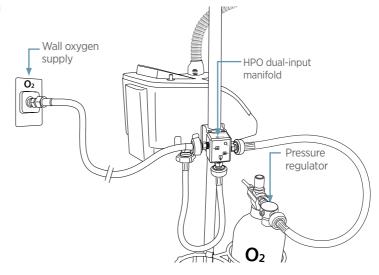

The HPO dual-input manifold will use the oxygen-bottle supply automatically. Check the battery contains enough charge for intra-hospital transport. A new battery will provide therapy for approximately 40 minutes when fully charged. A Low Battery alarm will occur when 35% of the battery is remaining (no changes to the device or therapy). A Critically Low Battery alarm will occur when 20% of the battery is remaining (humidity is turned off, oxygen and flow continue to be delivered). When the battery is fully depleted, the Airvo 3 will interrupt therapy and produce a Power Out alarm.

- 3. Unplug the Airvo 3 from the wall power supply.
- 4. The Airvo 3 will display a Battery Mode: Low Humidity alarm.
- 5. When you reach your destination:
 - Reconnect the Airvo 3 to the wall power supply and the wall oxygen vlagus.
 - Turn off the oxygen bottle pressure regulator to avoid draining the oxygen bottle and switch to the wall oxygen supply.

If you are not using the HPO dual-input manifold, connect an oxygen bottle (if required) to one of the oxygen inlet ports when transporting your patient. Ensure any oxygen supply connected to the low-pressure oxygen (LPO) inlet port is turned off when the device is in standby mode, not delivering therapy.





Warnings

Only use the Airvo 3 battery with the Airvo 3 device.

Only charge the Airvo 3 battery with the Airvo 3 device.

Loss of power will result in loss of therapy. In the event of a Critically Low Battery alarm, promptly connect the Airvo 3 to the wall power supply to avoid loss of therapy due to the battery becoming depleted.

Contact technical personnel to remove the battery from the device if it is not likely to be used for an extended period of time.

5.6 Stopping therapy



When therapy is finished:

- 1. Remove the patient interface from your patient.
- 2. If oxygen is provided through the low-pressure oxygen inlet port on the top of the Airvo 3, turn off and disconnect the oxygen supply.

The Airvo 3 will automatically stop oxygen provided through the highpressure oxygen inlet port. You do not need to disconnect it.

- 1. Tap the STOP button to end therapy.
- 2. Review any warnings, then tap Yes to confirm and enter standby mode or No to continue therapy.
- 3. Turn the Airvo 3 off by holding down the Power button for 2 seconds.
- 4. Tap Yes to power down the device.

The Airvo 3 must be cleaned and disinfected between patients. Follow the reprocessing instructions if your patient has finished using the device.



✓! Warning

To avoid burns, do not touch the heater-plate or the bottom of the water chamber. The water in the chamber and the heater-plate beneath the chamber become hot during use.

Turn off the low-pressure oxygen source before stopping therapy. The oxygen flow must be turned off when the Airvo 3 is not delivering therapy to ensure oxygen does not build up inside the device.

6. Monitoring data



/ Warning

In line with the indications for use of the Airvo 3, the monitoring functionality of the Airvo 3 is intended for use on spontaneously breathing patients and not intended for patients requiring life support. It is the responsibility of the clinician to select the appropriate level of monitoring for their patient and to be prepared to deal with alarms and equipment malfunction. Additional, independent monitoring equipment may be necessary.

The Airvo 3 records up to 24 hours of data for review on the Data and Graphs screen, accessible by tapping the Data and Graphs information button 🗠 from the Home screen. Data and Graphs data will be lost if power from the battery and from the wall power supply is lost. Refer to the Airvo 3 Technical Manual for detailed information on data handling.

The Airvo 3 is designed not to collect identifiable information about end-users. To function effectively, Airvo 3 will collect and store limited therapy data.


Limited Airvo 3 device information may be collected by F&P to monitor medical device performance, including device identifiers. This is to monitor medical device effectiveness, and improvement opportunities (e.g. firmware). Information is stored and used securely by F&P and does not include any data relating to your patient's personal information.

For more information about what type data is involved in these activities, refer to the Airvo 3 Technical Manual.

Please refer to the T&Cs for your data protection and privacy obligations. Alternatively, refer to our Global Privacy Statement on our website for more on how we handle personal information.

Data can be transferred from the Airvo 3 to data collection devices via the data port adapter. Integration with the data collection device is required.

The graph selector screen shows all of the available graphs for the therapy. A graph can be accessed by pressing on a tile. Graphs can alternatively be selected using the scroll button outside of the graph selector screen.





6.1 **Patient data**

The values displayed in the patient data screen are described below. Measurements that are not available are shown as "--". Measurements may not be available when the Airvo 3 is in standby mode or the device has not collected enough data for a reliable measurement



Label	Unit	Description
Flow L/min The current flow rate of breathing gases supplied to the patient		The current flow rate of breathing gases supplied to the patient
RR BPM The patient's respiratory rate (breaths per minute), averaged		The patient's respiratory rate (breaths per minute), averaged over the last 90 seconds
Humidity °C The current humidity of breath		The current humidity of breathing gases supplied to the patient
FiO ₂ % The current fraction of oxygen		The current fraction of oxygen in breathing gases supplied to the patient
SpO ₂ /FiO ₂		Ratio of SpO ₂ and FiO ₂
ROX		SpO ₂ divided by FiO ₂ and respiratory rate
SpO ₂ % Peripheral blood oxygen saturation measured		Peripheral blood oxygen saturation measured by pulse oximeter
PR	BPM	Pulse rate measured by pulse oximeter (beats per minute)

6.2 Live value graphs

Airvo 3 live value trends graphs show the last 30 seconds of data.

Label	Unit	Description
Flow	L/min	The current flow rate of breathing gases supplied to the patient

6.3 Long term graphs

Airvo 3 Data and Graphs show measurements plotted against time for up to 24 hours. New measurements are added to the right side of the graph. Prior data will scroll to the left as new measurements are added. Gaps will appear in the plotted data if therapy is stopped or measurements are missing due to poor signal quality.

The graphs available are described in the table below.

Label	Unit	Description
Target flow L/min The target flow rate of br		The target flow rate of breathing gases supplied to the patient
RR BPM The patient's respiratory rate (breaths per minute), averaged over the las		The patient's respiratory rate (breaths per minute), averaged over the last 90 seconds
FiO ₂ % The fraction of oxygen in breathing gases supplied to the patient		The fraction of oxygen in breathing gases supplied to the patient
SpO ₂ /FiO ₂		Ratio of ${\rm SpO_2}$ and ${\rm FiO_2}$
ROX		${\rm SpO_2}$ divided by ${\rm FiO_2}$ and respiratory rate
SpO ₂	%	Peripheral blood oxygen saturation measured by pulse oximeter
PR	BPM	Pulse rate measured by pulse oximeter (beats per minute)

7. Troubleshooting

This section describes common causes, and solutions to, problems and alarms that you may encounter while using the Airvo 3. The Airvo 3 Technical Manual contains additional information that may be helpful in resolving more advanced problems.

7.1 **Alarms**

The Airvo 3 has visual and auditory alarms to notify users about interruptions to a patient's treatment. These alarms are generated by an intelligent alarm system, which processes information from sensors and target settings of the device and compares this information with pre-programmed limits. Changes to alarm settings will be preserved during or after any power loss.

The signal light flashes and troubleshooting information is displayed on the Airvo 3 touch screen when any alarm is active. The color of the signal light indicates the highest-priority active alarm condition.



7.2 **Alarm priority**

Alarms are grouped by urgency and severity into three priority levels: low, medium, high. When multiple alarms are active, the audible alert, signal light and Message bar background color will signal the highest-priority alarm active.

- · A response is needed for all alarms.
- A prompt response is required for all medium-priority alarms.
- · An immediate response is required for all high-priority alarms.

Priority Message bar, signal light color		Audible alert
Low	Solid yellow	High then low-pitched beep
Medium	Flashing yellow	3 beeps every 9 seconds
High	Flashing red	10 beeps every 5 seconds



Audible alarms may not be heard if the alarm volume is set lower than ambient noise. Missed alarms may lead to patient injury. Refer to the Airvo 3 Technical Manual to review and set the alarm volume.

7.3 **Auditory information signals**

The informative sounds made by the Airvo 3 are:

Melody	Meaning
Ascending sequence of 5 tones	The breathing gas has warmed up
Single tone	A touch on the display has been registered
Single low then high tone	All active alarms have been resolved
High note followed by 2 (identical) lower notes, repeated every 10 seconds	The Power Out alarm is active. The wall power supply has been disconnected or turned off and the (optional) battery is depleted
Descending sequence of 3 tones	The device has completed the power off process
Sequence of 3 tones with high, low then middle pitch	The device has been turned on

Viewing alarm details 7.4

Alarms are displayed with suggestions and action buttons for managing the alarm information:

- Tap the Audio Pause button to silence the alarm for 120 seconds. The Audio Pause button will change to when audible alarms are silenced.
- Use \(\rightarrow \tag{to scroll through multiple suggestions.} \) Some alarms have only one suggested resolution.
- Tap Hide suggestions to collapse the alarm information to the Message bar. Restore suggestions by tapping the alarm condition on the Message bar.

The alarm condition and action button are displayed on the Message bar when alarm information is collapsed.

The Message bar cycles through each alarm condition when multiple alarms are active. Tapping the Message bar displays a list of active alarm conditions, from highest priority to lowest priority and they are ordered from when they occurred.

Alarm signals always indicate the highest-priority active alarm condition.


Checking the alarm system 7.5


To test the alarm system:


- In standby mode, disconnect the breathing tube then press "Start".
- 2. Verify that the "Check tube" visual alarm appears on screen.
- 3. Verify that the signal light flashes yellow.
- 4. Verify that the auditory alarm signal can be heard

Do not use the Airvo 3 if it fails this test. Contact your Fisher & Paykel Healthcare representative.

7.6 Airvo 3 alarms

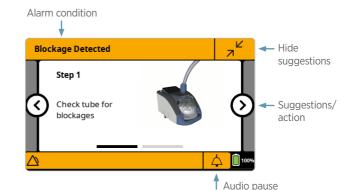



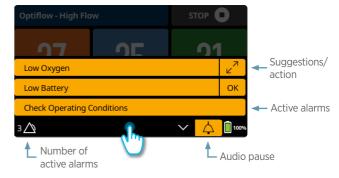

120 seconds and the signal light above the touch screen will flash. The touch screen is off during the Power Out alarm. The Airvo 3 will shut down after signaling the Power Out alarm but will restart automatically if power is restored

All the alarms you may encounter while using the Airvo 3 are listed below with common causes, resolutions and any delays inherent in determining alarm conditions. These priorities have been allocated for an intended operator's position of 2 meters from the device. The Airvo 3 also uses an internal-priority ranking system. If multiple alarm conditions occur simultaneously, the device will display the highest-priority alarm.

Alarm condition	Priority	Delay	Meaning
Faults			
Device Fault [Fault X.X.X]	High	-	A technical fault has occurred that has caused therapy to be stopped. Restart the device to resolve the fault. If the issue persists, contact your service representative.
Device Fault [Fault X.X.X]	Med.	-	A technical fault has occurred, and the device is able to continue supplying limited therapy. Restart the device to resolve the fault. If the issue persists, contact your service representative.
Power alarms			
Power Out	High	< 5 s	The Airvo 3 has been disconnected from the wall power supply and the internal battery is depleted. The auditory alarm will sound once every 10 seconds for

before it shuts down.

Alarm condition	Priority	Delay	Meaning
Unsupported Battery	Med.	<5s	The device is running off the battery and either an incorrect battery type is connected or communications with the battery could not be established. Charging is disabled. During battery use the behaviour is the same as the Critically Low Battery alarm.
Critically Low Battery	Med.	< 5 s	The Airvo 3 battery level is critically low and indicates at least 5 minutes left for complete loss of battery power. The humidification is turned-off to maintain operation of the blower and oxygen supply. Connect to wall power supply to continue therapy as normal.
Low Battery	Low	< 5 s	The Airvo 3 battery level is low and indicates at least 10 minutes left for complete loss of battery power. Connect to wall power supply to continue therapy as normal.
Battery Mode: Reduced Humidity	Low	< 5 s	The Airvo 3 has been disconnected from the wall power supply and the device is now running off the battery. The delivered humidity may be reduced.
Battery Charger Fault	Low	< 30 s	The battery charger is not functioning correctly and has been disabled. Restart the device to resolve the fault. If the issue persists, contact your service representative.
Therapy alarm - tube			
Outlet Elbow Missing	High	< 15 s	The Airvo 3 outlet elbow has been removed from the device during therapy. Check that the outlet elbow is fully inserted into the Airvo 3. If the issue persists, replace the outlet elbow.
Check Tube	Med.	< 5 s	The Airvo 3 cannot detect the heated breathing tube. Check that the heated breathing tube is not damaged and is plugged in correctly. Replace the heated breathing tube if the problem persists.
Wrong Tube	Med.	< 5 s	The heated breathing tube is not suitable for the selected therapy, or is damaged. Connect a suitable heated breathing tube. Replace the breathing tube if the problem persists.
Outlet Elbow Fault	Med.	< 5 s	A fault has been detected with the outlet elbow. Check that the outlet elbow is fully inserted into the Airvo 3. If the issue persists, replace the outlet elbow.
Outlet Elbow Too Warm	Med.	< 5 s	The outlet elbow is too warm to run start up checks. Wait for the outlet elbow to cool down. If the issue persists, replace the outlet elbow.
Therapy alarm – high flow	N		
Chamber Leak Detected	Med.	< 30 s	The water chamber has been removed. Ensure the water chamber is correctly inserted into the Airvo 3. If the issue persists, contact your service representative.
Leak Detected	Med.	< 30 s	When used with Optiflow Junior 2 patient interfaces, the Airvo 3 has detected a leak in the breathing circuit. Check: the water chamber has not been removed and is properly installed, the heated breathing tube is plugged in correctly or is not damaged, the patient interface is fitted correctly, and the air filter is fitted correctly. If the issue persists, replace the consumables.
Blockage Detected	Med.	< 15 s	 The Airvo 3 has detected a blockage. Check: for blockages in the heated breathing tube, patient interface and inlet air filter, the patient interface is the correct size for the patient, and the target flow rate is within the rated range of the interface. If the issue persists, replace the consumables.

Alarm condition	Priority	Delay	Meaning
Flow Below Target	Med.	< 2 min	 The Airvo 3 flow rate is lower than the target flow rate. Check: for blockages in the heated breathing tube, patient interface and inlet air filter, the patient interface is the correct size for the patient, and the target flow rate is within the rated range of the interface. If the issue persists, replace the consumables.
Flow Above Target	Low	< 2 min	The Airvo 3 flow rate is higher than the target flow rate. Check: • for leaks in the water chamber, heated breathing tube and patient interface, • the inlet air filter is inserted correctly, and • the target flow rate is within the rated range of the interface. If the issue persists, replace the consumables.
Therapy alarm – other			
Target Flow Too High	Med.	< 60 s	 The Airvo 3 has exceeded an internal temperature limit. Continued operation in the current configuration may result in a device fault and reduced therapy Check: for blockages in the heated breathing tube, patient interface and inlet air filter, the patient interface is the correct size for the patient, the target flow rate is within the rated range of the interface, and the ambient temperature is within the rated range of the device. This alarm will resolve when the internal temperature is within the expected
Check Water	Med.	< 30 min	range. The water chamber has run out of water. Replace the water bag to resume normal operation. Ensure that the water chamber and/or water bag are not allowed to run out of water to ensure continuous humidification of the breathing gases.
Humidity Below Target	Low	< 30 min	The Airvo 3 cannot reach the target humidity. Check the water chamber contains water and the chamber base is not damaged. Consider reducing the target humidity or flow rate, if appropriate. If the issue persists, replace the water chamber.
Check Operating Conditions	Low	< 1 min	The Airvo 3 has detected ambient conditions that are not suitable. Do not use the Airvo 3 when the ambient temperature is below 18 °C or above 28 °C. Move the device to a suitable environment.
Oxygen alarms			
No O ₂ Pressure at HPO Port	Med.	< 5 s	There is no oxygen being supplied to the high-pressure (HPO) inlet port during therapy. Check that the oxygen supply is working. If using an oxygen bottle, check the bottle is not empty. If switching to the low-pressure (LPO) inlet port or stopping oxygen delivery, set the ${\rm FiO_2}$ target to 21 %.
FiO ₂ Below 25%	Med.	< 30 s	The oxygen being supplied to the LPO port has fallen below 25% during therapy. Check if the oxygen supply has been disconnected.
FiO ₂ Below Target	Med.	< 2 min	The oxygen concentration being delivered is lower than the FiO2 target setting. Check the oxygen supply is properly connected to the HPO inlet port and there are no leaks at any oxygen hose connections. Make sure the number of connected devices does not exceed the capacity of the oxygen supply. Consider using the LPO connection if the oxygen supply has insufficient capacity.
FiO₂ Above Target	Med.	< 2 min	The oxygen concentration being delivered is higher than the ${\rm FiO_2}$ target setting. Check an oxygen supply is not connected to the low-pressure oxygen inlet port. Only one oxygen source should be used at a time. Check the oxygen supply is properly connected to the high-pressure oxygen inlet port and that there are no leaks at the oxygen hose connections.

Alarm condition	Priority	Delay	Meaning
High FiO₂ (LPO)	Med.	< 20 s	The FiO_2 supplied by the LPO port is above the selected High Oxygen Alarm threshold for its intended clinical environment (range 30-95% or Off, default: 95%, see Airvo 3 Technical Manual). Check FiO_2 is appropriate for the patient's condition. Reduce FiO_2 to the normal range when it is appropriate to do so.
Unexpected O ₂	Med.	< 15 min	Oxygen is being supplied to the Airvo 3 while in standby. Check all oxygen supplies are turned off and disconnected. If the issue persists, contact your service representative.
High FiO₂ (HPO)	Low	< 5 s	The FiO $_2$ target is above the selected High Oxygen Alarm threshold for its intended clinical environment (range 30-95% or Off, default: 95%, see Airvo 3 Technical Manual). Check FiO $_2$ is appropriate for the patient's condition. Reduce FiO $_2$ to the normal range when it is appropriate to do so.
Pulse oximetry alarms			
Pulse Ox Communication Failure	Med.	< 10 s	The Airvo 3 is unable to communicate with the pulse oximeter. Check that the USB connector cable, sensor adapter cable and sensor cables are all properly connected. Replace the sensor cable, adapter cable then USB connector cable in turn if the problem persists.
Pulse Ox Not Recognized	Med.	< 10 s	The selected pulse oximeter has not been recognised. Please remove or change oximeter.
Pulse Ox Disconnected	Med.	<1s	The pulse oximetry USB connector cable has become disconnected. Reconnect pulse oximetry USB connector cable.
No Pulse Ox Sensor Connected	Med.	<1s	A pulse oximetry sensor cable was not detected or is inoperable. Check that the sensor cable is properly connected to the USB connector cable or replace the sensor cable if necessary.
Pulse Ox Sensor Off Patient	Med.	<1s	The pulse oximeter is no longer receiving ${\rm SpO_2}$ measurements from the patient. Check that the sensor is properly attached to a suitable measurement site on the patient.
No SpO ₂ Reading	Med.	<1s (Masimo and Nellcor)	The pulse oximeter is not sending valid ${\rm SpO_2}$ measurements. Check the sensor, cable and USB interface. Try replacing each component in turn until the problem is resolved.
		< 16 s (Nonin)	
No Pulse Rate Reading	Med.	<1s (Masimo and Nellcor)	The pulse oximeter is not sending valid Pulse Rate measurements. Check the sensor, cable and USB interface. Try replacing each component in turn until the problem is resolved.
		< 16 s (Nonin)	
Check Pulse Ox Cable/ Sensor	Med.	<1s	Masimo only . The pulse oximetry USB connector cable and/or the pulse oximetry sensor cable is not functioning correctly. Please remove and reconnect the accessory and if the problem persists replace the accessory.
Incompatible Pulse Ox Cable	Low	<1s	Masimo only. The pulse oximetry USB connector cable is incompatible. Please disconnect it from the device.
Incompatible Pulse Ox Sensor	Low	<1s	Masimo only. The pulse oximetry sensor cable is incompatible. Please disconnect it from the device.
Pulse Ox Cable Near Expiration	Low	<1s	Masimo only. The pulse oximetry USB connector cable is nearing expiration.
Pulse Ox Sensor Near Expiration	Low	<1s	Masimo only. The pulse oximetry sensor cable is nearing expiration.
Pulse Timeout	High	<1s	Nellcor only . The pulse oximetry USB connector cable is reporting the loss of a patients pulse signal. Check the condition of the patient.


Alarm condition	Priority	Delay	Meaning
SpO₂ Measurement Delayed	Low	<1s	Nellcor only. The pulse oximeter is indicating that its dynamic averaging time has exceeded 25 seconds for the SpO_2 measurement.
Pulse Rate Measurement Delayed	Low	<1s	Nellcor only. The pulse oximeter is indicating that its dynamic averaging time has exceeded 25 seconds for the pulse rate measurement.
Pulse Ox Board Failure	Med.	<1s	Masimo and Nellcor only . The pulse oximetry USB connector cable has failed. Please remove and reconnect the cable and if the problem persists replace the cable.
Check Pulse Ox Sensor	Med.	<1s	Masimo and Nellcor only. The pulse oximetry sensor cable is not functioning correctly. Please remove and reconnect the cable and if the problem persists replace the cable.
Replace Pulse Ox Cable	Med.	<1s	Masimo and Nellcor only. There is a fault with the pulse oximetry USB connector cable and it needs replacement.
Replace Pulse Ox Sensor	Med.	<1s	Masimo and Nellcor only. There is a fault with the pulse oximetry sensor cable and it needs replacement.
Physiological alarms			
Low SpO ₂	High	< 15 s	Check your patient. The ${\rm SpO}_2$ measurement has decreased below the Low ${\rm SpO}_2$ alarm threshold. Check that the alarm setting is appropriate for your patient (Range: 1-98%, default 85%, see Airvo 3 Technical Manual).
High SpO₂	Med.	< 15 s	Check your patient. The SpO_2 measurement has exceeded the High SpO_2 alarm threshold. Check that the alarm setting is appropriate for your patient (Range: 2-99% or Off, default Off, see Airvo 3 Technical Manual).
Disinfection alarms			
Disinfection Failed to Hold Temperature	Med.	< 3 min	 The Airvo 3 cannot heat up to the required disinfection temperature. Check: the disinfection tube blue connector is connected to the top of the outlet elbow, the disinfection tube red end is connected to the left hand chamber port, the disinfection filter is connected to the right hand chamber port,
			Then restart the device. If the problem is not resolved, replace the disinfection tube and outlet elbow in turn. If the issue persists, contact your service representative.
Over Temperature Detected	Med	<5 s	 The Airvo 3 detected higher than expected temperatures during the disinfection cycle. Check: the disinfection tube blue connector is connected to the top of the outlet elbow, the disinfection tube red end is connected to the left hand chamber port,
			 the disinfection filter is connected to the right hand chamber port, Then restart the device. If the problem is not resolved, replace the disinfection tube and outlet elbow in turn. If the issue persists, contact your service representative.
Check Tube	Med.	<5 s	The Airvo 3 cannot detect the disinfection tube. Check that the disinfection tube is not damaged and is plugged in correctly, then restart the device. If the problem is not resolved, replace the disinfection tube and outlet elbow in turn. If the issue persists, contact your service representative.
Leak Detected	Med.	<35 s	 The Airvo 3 has detected a leak in the disinfection circuit. Check: The disinfection tube blue connector is connected to the top of the outlet elbow, The disinfection tube red end is connected to the left hand chamber port, The disinfection filter is connected to the right hand chamber port,
			Then restart the device. If the problem is not resolved, replace the disinfection tube and outlet elbow in turn. If the issue persists, contact your service representative.

Alarm condition	Priority	Delay	Meaning
Blockage Detected	Med	<10 s	The Airvo 3 has detected a blockage. Check that the disinfection tube is not blocked and that the disinfection filter is not wet, then restart the device. If the problem is not resolved, replace the disinfection tube and outlet elbow in turn. If the issue persists, contact your service representative.
Check Operating Conditions	Med.	<1 min	The Airvo 3 has detected ambient conditions that are not suitable. Do not use the Airvo 3 when the ambient temperature is below 18 °C or above 28 °C. Move the device to a suitable environment, then restart the device. If the issue persists, contact your service representative.
Wall Power Disconnected	Med.	< 5 s	The power cable has been removed and device is unable to perform a disinfection cycle. Connect device to wall power, then restart the device. If the issue persists, contact your service representative.
Unexpected O ₂	Med.	<1 min	Oxygen is being supplied to the Airvo 3 while in disinfection mode. Check all oxygen supplies are turned off and disconnected. If the issue persists, contact your service representative.

8. Reprocessing

Standard aseptic techniques should be followed to minimize contamination when handling the Airvo 3 and accessories. The patient interface, heated breathing tube, water chamber and outlet elbow may become contaminated during use. As soon as possible after using the Airvo 3:

- 1. Remove the single-use accessories from the Airvo 3 and dispose of them in accordance with local laws, regulations and hospital protocols for disposing of contaminated products.
 - Squeeze the sides of the breathing tube connector and lift to remove it from the Airvo 3.
 - Grip the port adapter and pull the water chamber away from the Airvo 3 to remove it.

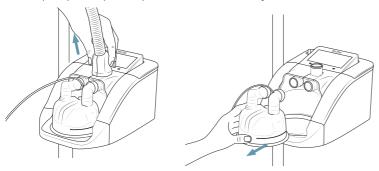

- 2. Reprocess the Airvo 3 device exterior by following the instructions in section 8.1.
- 3. Clean and high-level disinfect the Outlet Elbow by following the instructions in section 8.2.
- 4. Replace accessories within the maximum use period shown in section 8.3 (schedule for changing accessories).
- 5. Clean and disinfect pulse oximetry accessories (including reusable sensors) in accordance with the manufacturer's instructions.



Warnings

Do not clean and/or disinfect the Airvo 3 while it is being used by a patient.

Do not submerge the Airvo 3 or accessories in any cleaning solution or attempt to sterilize by autoclave, irradiation, steam, gas, ethylene oxide or any other method. This will seriously damage the device.

8.1 Airvo 3 device exterior reprocessing

8.1.1 Clean

Equipment

- · Mild detergent
- · Clean, disposable, lint-free cloths
- Protective gloves

Cleaning Instructions

- 1. Mix a solution of warm water and mild detergent (refer to the detergent manufacturer's instructions for use).
- 2. Dampen a clean cloth with the cleaning solution.
- 3. Thoroughly wipe all outside surfaces of the device (including the Outlet Elbow) for at least one minute to remove any visible soil. Use the corner/edge of the cloth to clean all crevices of the device.

Rinse

- 4. Dampen a clean cloth with tap water.
- 5. Thoroughly wipe all outside surfaces of the device with the damp cloth to remove any disinfectant residue.

Drv

- 6. Thoroughly wipe all outside surfaces of the device with a dry cloth until it is visibly dry.
- 7. Allow to air dry until completely dry.

8.1.2 Disinfect

Perform disinfection only after all cleaning steps are complete

Equipment

- · Disinfectant wipes
- · Clean, disposable, lint-free cloths
- Protective gloves

Disinfection Instructions

- 1. Use pre-soaked disinfecting wipes, to thoroughly wipe all outside surfaces of the device (including the Outlet Elbow).
- 2. Ensure that these surfaces remain visibly wet as directed by the manufacturer of the disinfecting wipes. Use additional wipes as needed to ensure that these surfaces remain wet for the required length of time.

Rinse

- 3. Dampen a clean cloth with tap water.
- 4. Thoroughly wipe all outside surfaces of the device with the damp cloth to remove any disinfectant residue.

Dry

- 5. Thoroughly wipe all outside surfaces of the device with a dry cloth until it is visibly dry.
- 6. Allow to air dry until completely dry.



✓! Warnings

Other cleaning agents may be used if they are: non-abrasive, non-toxic, and non-corrosive. Do not use any cleaning agents that are not compatible with polycarbonate plastic.

Cleaning agents that are not suitable for use with the Airyo 3 include: ammonia, ammonium hydroxide, caustic soda, iodine, methanol, methylated spirits, turpentine, and alkaline bleaches such as sodium hypochlorite. The use of any of these products will damage the Airvo 3.

Turn off and disconnect the Airvo 3 from the wall power supply before cleaning to reduce the risk of electric shock.

Do not submerge the device in liquid of any kind.

Do not spray liquid directly onto the device.

Do not use rinse aids as these may cause damage to the outlet elbow.

These instructions have been validated by the manufacturer of the medical device as being capable of preparing a medical device for reuse. It remains the responsibility of the processor to ensure that the processing achieves the desired results, by using the correct equipment, materials, and personnel in the processing facility. This requires routine monitoring of the process.

Outlet elbow reprocessing

The Outlet Elbow requires cleaning and high-level disinfection. The Outlet Elbow can be reprocessed in two different ways:

- Disinfection Kit 900PT600 (see instructions in 900PT600)
- Washer-Disinfector (follow below instructions)

The outlet elbow can be removed from the Airvo 3 for reprocessing by your central sterile services or reprocessing department. Reprocessing the outlet elbow must be performed in a washer-disinfector that complies with and is maintained, checked and validated to ANSI/AAMI ST15883-1:2009 (USA) and ISO 15883-1:2006 (outside USA).

Disassembly

Remove the outlet elbow from the Airvo 3. Firmly grab the rubber port-seal on the outlet elbow, push down on the grip lines with your thumb and pull the outlet elbow towards the front of the Airvo 3.



Transportation


Follow hospital infection control protocols to package the outlet elbow for transport. Protect the outlet elbow from mechanical damage during transport.

Using the storage cover

It is important that the Airvo 3 is stored properly after reprocessing. Store the Airvo 3 in a clean, dry and dust-free location that is suitable for medical devices.

Cover the Airvo 3 with the storage cover so that it remains clean during storage:

- Wrap the Airvo 3 in a storage cover (900PT603) so that the identification label on the cover sits prominently above the display of the Airvo 3.
- Seal the cover with the adhesive tabs on the storage cover.



Cleaning and disinfection

Washer-disinfector supplies required for reprocessing of the Airvo 3 outlet elbow are:

Mildly alkaline cleaning agent such as neodisher® MediClean forte (0.2% v/v)

Place the outlet elbow in a washer-disinfector and orient the outlet elbow such that washing fluid can contact all internal surfaces and allow for draining. Run a cleaning and thermal high-level disinfection cycle:

- Pre-cleaning: Cold rinse for at least 1 minute
- Cleaning: Wash at 55 °C for at least 5 minutes with a mildly alkaline cleaning agent as per manufacturer's instructions (e.g. neodisher*) MediClean forte, 0.2 % v/v)
- · Neutralisation: Cold rinse for at least 1 minute
- Rinsing: Cold rinse for at least 1 minute
- Thermal disinfection: 90 °C for 5 minutes
- · Drying: 90 °C for 25 minutes



Do not exceed the maximum use period for the outlet elbow.

Follow the manufacturer's instructions and warnings for all cleaning products.

Visual inspection

Visually inspect the outlet elbow for mechanical damage or discoloration of the chamber seal. If the seal or elbow appear damaged or discolored, replace the outlet elbow.



Warning

Do not use the outlet elbow if the seal or elbow appear damaged or discolored. A damaged outlet elbow may affect therapy delivery.

Storage and transport

It is important that the outlet elbow is stored properly after reprocessing. Store the outlet elbow in a clean, sealed plastic bag labeled with the disinfection process details. Follow your hospital protocol for storage of high-level disinfected devices. Protect the outlet elbow from mechanical damage during transport. Store the outlet elbow in a clean, dry and dust-free location that is suitable for medical devices. The outlet elbow can alternatively be inserted back into the Airvo 3 then covered with the storage cover until the next use.

Reassembly

When setting up the Airvo 3 for the next use follow the reassembly steps below. If reassembly occurs prior to the next use, cover the Airvo 3 with the outlet elbow assembled with the clean storage cover.

Slide the disinfected outlet elbow into the slot above the chamber area on the Airvo 3.

Push firmly on the front of the elbow until the elbow locks into place.



Make sure the outlet elbow is installed in the Airvo 3 before attaching the heated breathing tube.



8.3 **Schedule for changing accessories**

The Airvo 3 accessories must be changed according to the schedule below. All single-patient-use accessories must be disposed of after the patient's therapy to prevent cross-contamination. Replace accessories within the period shown below, or immediately if they are damaged or discolored.

Maximum use
1 week, or 1 patient (whichever comes first)
14 days (7 days when using a nebulizer), or 1 patient (whichever comes first)
3 months or 1000 hours use (whichever comes first)
5 years or 50 washer-disinfector cycles (whichever comes first)
2 years from first use or 300 discharge cycles (whichever comes first)
Refer to instructions for use supplied with device

^{*} See Airvo 3 Technical Manual for instructions to change the battery.

8.4 Replacing the air filter

The Airvo 3 will display a message on startup when the air filter is due to be replaced.


Begin by removing the old filter:

- 1. Raise the filter cover.
- 2. Push the filter removal tool down firmly onto the low-pressure oxygen inlet port to get the removal tool to grip.
- 3. Hold down the air-filter release button.
- 4. Pull up on the filter removal tool to remove the filter.
- 5. Insert the new filter and push down on top of the filter until it clicks into place.
- 6. Lower the filter cover.

8.5 Servicing

The Airvo 3 does not require regular maintenance and contains no user serviceable parts. If the Medical Equipment system is modified from the specification of the manufacturer, evaluation to the requirements of 60601-1 standard is required. Refer to the Airvo 3 Technical Manual for product acceptance checks, functional tests and spare parts. Contact your Fisher & Paykel Healthcare representative if a fault develops or you are concerned the Airvo 3 is not operating correctly.





9. Pulse oximetry

The Airvo 3 supports the following pulse oximeter accessories:

- The Masimo SET uSpO₂ Pulse Oximetry Cable (3412)
- The Medtronic Nellcor Oxicable (PMC10N-SF)
- The Nonin Xpod 3012LP USB (6703-001)
- The Nonin Xpod 3012HR USB Connector Cable (114403-001)

Pulse oximeters primarily measure the oxygen saturation of blood and pulse rate. Oxygen saturation or SpO₂ is the percentage of hemoglobin in the blood that is saturated with oxygen. Hemoglobin is a protein in the red blood cells that carries oxygen from the lungs to the rest of the body. Pulse rate is the number of heart beats per minute.

A pulse eximeter operates by emitting two different wavelengths of light, typically red and infrared, into a perfused tissue site such as a fingertip or earlobe. The emitted light passes through the tissue, and a photodetector in the sensor measures the intensity of the transmitted or reflected light. By comparing the absorption of red and infrared light, the pulse oximeter calculates the ratio of oxygenated to total hemoglobin in the blood, which is used to determine the oxygen saturation level. Additionally, the device analyzes the variations in the light intensity to measure the patient's pulse rate.

Pulse oximetry warnings, cautions, and notes



🔼 Warnings

- In line with the indications for use of the Airvo 3, the monitoring functionality of the Airvo 3 is intended for use on spontaneously breathing patients and not intended for patients requiring life support. It is the responsibility of the clinician to select the appropriate level of monitoring for their patient and to be prepared to deal with alarms and equipment malfunction. Additional, independent monitoring equipment may be necessary.
- If any measurement seems guestionable, first check the patient's vital signs by alternate means and then check the pulse oximeter for proper functioning.
- Using different alarm settings on devices within a single area, such as an intensive care unit, can cause a hazard.
- Periodically reposition the sensor to help prevent ischemia.
- If any measurement seems questionable, first check the patient's vital signs by alternate means. Then check the pulse oximeter USB connector, adapter, sensor, and Airvo 3 for proper operation.
- Carefully route cabling to reduce the possibility of patient entanglement or strangulation.
- Do not use single-patient-use pulse oximeter sensors on more than one patient to avoid cross-infection and/or contamination.
- Refer to the third party pulse oximeter sensor instructions for information on the risks of re-using a single use sensor.
- Follow the user instructions supplied with multi-use pulse oximeter sensors, adapters and USB connector cables to clean and disinfect these devices between patients to avoid cross-infection and/or contamination.
- Tissue damage may be caused by incorrect application of the sensor, e.g. by wrapping the sensor too tightly. Follow the instructions supplied with the sensor for correct application.
- Use only compatible oximetry sensors and accessories for SpO₂ and pulse rate measurements. Verify compatibility before use to avoid incorrect operation of your Airvo 3, inaccurate measurements and/or patient injury. See Appendix 3 for a list of compatible
- Supplemental oxygen will attenuate patterns of desaturation. A patient's respiratory compromise can be proportionally more severe before patterns appear in the saturation trend. Remain vigilant when monitoring a patient on supplemental oxygen.
- Explosive hazard: Do not use this device in an explosive atmosphere or in the presence of flammable anesthetics or gases.
- To protect from electric shock, always remove the sensor and completely disconnect the pulse oximeter before bathing the patient. Nellcor:
- Do not rely solely on the Nellcor Oxicable for patient assessment. It must be used in conjunction with clinical signs and symptoms.
- Avoid spilling liquids into the Nellcor Oxicable.
- Refer to the Oxicable PMC10N-SF instructions for use for a complete list of warnings and more information when using the Medtronic Oxicable with the Airvo 3.

Nonin:

Operation of the Nonin Xpod USB connector below the minimum amplitude of 0.3% modulation may cause inaccurate results.

∠!\ Cautions

- Before cleaning the pulse oximetry accessories, disconnect the device from the Airvo 3 to avoid electrical shock and flammability
- Do not place the pulse oximetry accessories on electrical equipment that may affect the device, preventing it from working properly.
- To minimize radio interference, other electrical equipment that emits radio frequency transmissions should not be in close proximity to the pulse oximeter equipment.
- Do not place the Airvo 3 where controls can be changed by the patient.
- The accuracy of the SpO₂ measurement may be affected if the total sensor cable length (including extension cables) is greater than 3 meters.
- · Setting extreme alarm thresholds can render alarms useless and may lead to patient injury.
- · Check that the pulse oximetry alarm limits are appropriate for the patient being monitored every time pulse oximetry is used.

• Inspect the sensor application site at least every 6 to 8 hours to ensure correct sensor alignment and skin integrity. Patient sensitivity may vary due to medical status or skin condition. Discontinue use of adhesive tape sensors if the patient exhibits an allergic reaction to the adhesive material.

Masimo:

- If the Low Perfusion message is frequently displayed, find a better perfused monitoring site. In the interim, assess the patient and, if indicated, verify oxygenation status through other means.
- Change the application site or replace the sensor and/or patient cable when a "Replace Pulse Ox Sensor" and/or "Replace Pulse Ox Cable", or a persistent poor signal quality message (such as "Low Signal I.Q") is displayed on the Airvo 3. These messages may indicate that patient monitoring time is exhausted on the patient cable or sensor.
- If using pulse oximetry during full body irradiation, keep the sensor out of the radiation field. If the sensor is exposed to the radiation, the reading might be inaccurate or the device might read zero for the duration of the active irradiation period.
- Variation in measurements may be profound and may be affected by sampling technique as well as the patient's physiological conditions. Any results exhibiting inconsistency with the patient's clinical status should be repeated and/or supplemented with additional test data. Blood samples should be analyzed by laboratory instruments prior to clinical decision making to completely understand the natient's condition
- Replace the cable or sensor when a "replace sensor" or when a "low SIQ" message is consistently displayed while monitoring consecutive patients after completing the troubleshooting steps listed in this manual.
- Please refer to the instructions for use provided with the Masimo uSpO₂ Pulse Oximetry Cable for additional warnings, cautions, and
- The Masimo SET uSpO2 Pulse Oximetry Cable (Oximetry Cable) must be connected to the Airvo 3 for power, communication, display and alarm management.

Nonin:


The Nonin Xpod USB connector has motion tolerant software that minimizes the likelihood of motion artefact being misinterpreted as good pulse quality. In some circumstances, however, this device may still interpret motion as good pulse quality. This covers all available outputs (i.e. SpO₂, PR, PLETH, PPG).

Note

- The accuracy of pulse oximeter sensors, adapters and patient cables cannot be assessed using a functional tester.
- High-intensity extreme lights (such as pulsating strobe lights) directed on the sensor, may not allow the pulse oximeter to obtain vital sign readings.
- When using the Maximum Sensitivity setting, performance of the "Sensor Off" detection may be compromised. If the device is in this setting and the sensor becomes dislodged from the patient, the potential for false readings may occur due to environmental "noise" such as light, vibration, and excessive air movement.
- For more information about required safety and regulatory requirements for pulse oximeters, refer to ISO 80601-2-61, and IEC 60601-1. Additional safety information can be found in the labelling provided with each sensor.
- Do not loop the pulse oximetry cabling into a tight coil or wrap around the device, as this can damage the patient cabling.
- Additional information specific to the sensors compatible with the Airvo 3 pulse oximeter, including information about parameter/ measurement performance during motion and low perfusion, may be found in the sensor's directions for use.
- Cables and sensors are provided with X-Cal™ technology to minimize the risk of inaccurate readings and unanticipated loss of patient monitoring. Refer to the Cable or Sensor directions for use for the specified duration of the patient monitoring time.
- Each specific sensor comes with manufacturer-supplied instructions for its use. Please refer to these for further details, including Bland Altman plots.

9.2 Setup for pulse oximetry

Connect the pulse oximetry USB connector cable to either USB port on the back of the Airvo 3. Clip the cable into the cable tidy so that it is not pulled out accidentally. The Airyo 3 will automatically detect a compatible pulse oximeter.

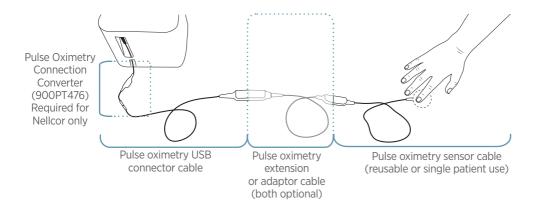

9.2.1 Pulse oximetry accessories

When compatible pulse oximetry accessories are connected, the Airvo 3 can display:

- functional oxygen saturation (SpO₂),
- pulse rate (no pulse rate alarms are included in the Airvo 3),
- perfusion index (Masimo only),
- · plethysmograph, and
- · signal quality indicators

9.3 During therapy


The Pulse Oximetry tile will be automatically displayed on the Home screen when a compatible pulse oximetry USB connector cable is connected to the Airvo 3.




Pulse oximetry measurements and status are shown as follows:



Tap the Pulse Oximetry tile to open the Pulse Oximetry screen.

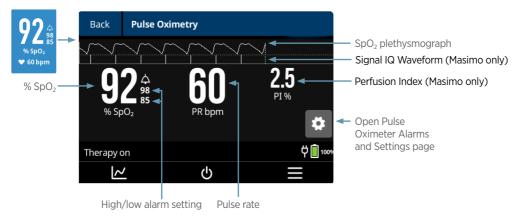



Connect the USB connector cable to the to Airvo 3

Connect the pulse oximeter USB connector cable to the USB port on the back of the Airvo 3. The Airvo 3 will automatically detect compatible devices. Connect the pulse oximetry sensor cable to the other end of the USB connector cable.



Attach sensor to patient

Carefully select a pulse oximetry sensor based on the patient's age, weight and intended sensor application site. More information can be found in the instructions supplied with each sensor.



✓!\ Warnings

Inaccurate SpO₂ and/or pulse-rate readings may be caused by:

- · Improper sensor application and placement.
- Elevated levels of Carboxyhemoglobin (COHb) or methaemoglobin (MetHb): High levels of COHb or MetHb may occur with a seemingly normal SpO₂ When elevated levels of COHb or MetHb are suspected, laboratory analysis (COOximetry) of a blood sample should be performed.
- · Elevated levels of bilirubin.
- · Elevated levels of dyshemoglobin.
- Vasospastic disease, such as Raynaud's, and peripheral vascular disease
- · Hemoglobinopathies and synthesis disorders such as thalassemia, Hb s, Hb c, and sickle cell, etc.
- Hypocapnic or hypercapnic conditions.
- · Severe anemia.
- · Very low arterial perfusion.
- · Extreme motion artifact.
- Abnormal venous pulsation or constriction.
- Severe vasoconstriction or hypothermia.
- · Arterial catheters and intra-aortic balloon.

- · Intravascular dyes, such as indocyanine green or methylene blue.
- Externally applied coloring and texture, such as nail polish, acrylic nails, glitter, etc.
- Birthmark(s), tattoos, skin discolorations, moisture on skin, deformed or abnormal fingers etc.
- Skin color disorders.
- · Excessive ambient light.
- · Excessive motion.
- Electrosurgical interference.
- Blood flow restrictors (arterial catheters, blood pressure cuffs, infusion lines, etc.).
- Moisture in the sensor.
- Improperly applied sensor.
- Incorrect sensor type.
- Poor pulse quality.
- · Venous pulsations.
- · Low haemoglobin concentrations.
- · A sensor not at heart level.

Dyes or any substance containing dyes that change usual blood pigmentation may cause erroneous readings.

Loss of monitoring can result if any objects hinder the pulse measurement. Ensure that no blood flow restrictors (e.g., blood pressure cuff) hinder pulse measurements.

The oximeter sensor may not work on cold extremities due to reduced circulation. Warm or rub the finger to increase circulation or reposition the sensor.

Inaccurate readings can result due to residue (e.g., dried blood) in light path or degradation of optical characteristics of sensor components. Refer to cleaning instructions supplied with the pulse oximetry accessories.

False high readings can result if SpO₂ is low due to dysfunctional hemoglobin (e.g. carboxyhemoglobin or methemoglobin).

Read the instructions supplied with the pulse oximetry accessories for additional safety information (including any potential risks or adverse effects from sensor materials), measurement site selection, detailed sensor setup, maximum sensor application time at a single site before repositioning, cable lifetime, sensor lifetime, factors that can interfere with measurement, troubleshooting and maintenance instructions.

9.4 Description of measurements

Pulse oximetry measurements are displayed on the Pulse Oximetry tile, the Pulse Oximetry screen and the Data and Graphs screen. Measurements are updated every second.


Tap the Pulse Oximetry tile to open the Pulse Oximetry screen and ∠ to open the Data and Graphs screen.

Tapping **O** on the Pulse Oximetry screen provides a shortcut to the pulse oximetry alarms and settings.

⚠ Caution

If any measurement seems questionable, check the patient's vital signs by another method. Then check the pulse oximetry accessories and Airvo 3 are set up, configured and working correctly.





Pulse Oximetry screen

9.4.1 SpO₂

The Airvo 3 is calibrated to display functional oxygen saturation (SpO₂) as a percentage. The SpO₂ value displayed is an average of measurements over a user selectable period (see Averaging Time in section 9.5 below). A long averaging period will generally produce more stable values but the SpO₂ displayed will respond more slowly to rapid changes in arterial blood oxygen saturation (SaO₂).

Stability of the SpO_2 measurements displayed may provide a good indication of a valid signal. Though stability is a relative term, experience with the device and patient observations will help you separate physiological effects from artifacts caused by a poorly-placed sensor or excess patient motion.

Inconsistencies between SpO₂ displayed on the Airvo 3 and arterial blood gas analysis or clinical assessment may be caused by:

- · poor signal quality,
- low perfusion,
- improperly-placed sensors or cables, and/or
- · the patient's condition.

9.4.2 Pulse rate

Pulse rate (, PR) measurements are based on optical detection of pulsatile peripheral blood flow by the pulse oximeter sensor. The pulse rate displayed, in beats per minute (bpm), is an average of measurements over a user-selectable period.

Small differences in the pulse rate displayed by different equipment may be caused by different approaches to averaging. Small discrepancies between cardiac electrical activity and pulse rate obtained from peripheral measurements can also arise. Large discrepancies between equipment may be caused by:


- · poor signal quality,
- · low perfusion,
- · improperly placed sensors or cables, and/or
- · the patient's condition.


9.4.3 Plethysmograph

A plethysmograph (or photo-plethysmograph) provides a non-normalized indication of the change in blood volume measured by the pulse oximeter sensor. The shape of the plethysmograph may change between patients, between measurement sites and for different sensor models. The plethysmograph provides an indication of signal inadequacy. A low amplitude or variable plethysmograph may indicate poor/inadequate signal. The plethysmograph is displayed on the Pulse Oximetry screen.









9.4.4 Signal IQ Waveform (Masimo)

The Signal IQ waveform shows the measurement confidence and timing of each detected pulse relative to the plethysmograph waveform. The height of the vertical bars indicate the relative confidence of the measurement. A high bar corresponds to higher confidence. In addition, the bars should visually correlate to the peak of the plethysmograph waveform. This along with perfusion index provides a better tool for assessing potential problems such as blood flow obstructions, poor sensor placement, artifacts or interference.

If Signal IQ is low an indication will occur with the status message "Low SpO₂ Signal IQ" displayed. During this time the SpO₂ and pulse rate numbers will be greyed out.

Pulse Oximetry Ö **ф** 🗓 100 Therapy on




9.4.5 Perfusion Index (Masimo)

The Perfusion Index (Pi) is the ratio of the pulsatile blood flow to the non-pulsatile or static blood in peripheral tissue. Perfusion index represents a noninvasive measure of peripheral perfusion that can be continuously and noninvasively obtained from a pulse oximeter.

9.4.6 Signal quality indicators (Nonin)

Nonin pulse oximetry equipment indicate signal quality based on the perfusion of the patient. There are three states: green, yellow, and red corresponding to high, low/marginal, and low/poor signal quality respectively. During these periods of low signal quality (signal inadequacy) pulse oximetry values displayed may be incorrect. The Airvo 3 indicates low signal quality by greying out the SpO₂ and Pulse rate numbers.



9.5 **Description of settings and alarms**


This section describes the behavior of pulse oximetry settings and alarms. See the Alarms and measurement section (9.6) on how to make changes to the alarm thresholds and settings.

Patient alarm thresholds

The following alarms can alert you to changes in your patient's condition:


- SpO₂ Low alarm
- SpO₂ High alarm

The corresponding alarm will be raised when a measurement is lower or higher than the alarm threshold. SpO₂ alarm thresholds are displayed on the Pulse Oximeter tile and Pulse oximeter screen.



9.5.2 SpO₂ Alarm Delay

The SpO₂ Alarm Delay setting defers the Low SpO₂ and High SpO₂ alarms for up to 15 seconds. This delay helps reduce non-actionable alarms for short desaturations. The alarm will start, if the alarm condition remains, after the delay.

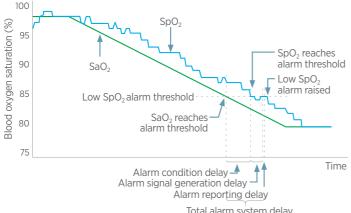

Total alarm system delay

9.5.3 Alarm response time

Audible and visual alarms are subject to an alarm response delay. The alarm response delay has three parts, the:

- 1. Alarm condition delay: the duration for a physiological change to be recognized by a pulse oximeter,
- 2. Alarm signal generation delay: the period between detecting a condition and signaling the alarm, and
- 3. Alarm reporting delay: the period between receiving an alarm signal from a monitoring device and reporting the alarm to the user.

Measurement averaging will affect the signal generation delay: a larger averaging time will increase the signal generation delay. These delay concepts are illustrated on the graph below for a decrease in SaO_2 leading to a SpO_2 Low alarm as an example. The illustration does not reflect the actual length of delays. Refer to ISO 80601-2-61 for more information about alarm response delay.

9.5.4 Averaging time

The SpO_2 averaging time can be adjusted depending on patient acuity and area of care. This is the time, in seconds for Masimo, and heart beats for Nonin that measurements are averaged over. Shorter averaging times are sometimes preferred in, for example, sleep testing while longer averaging times are more suited to telemetry and neonates.

9.5.5 Sensitivity modes (Masimo)

There are three sensitivity modes. Normal sensitivity is recommended for patients who are experiencing some compromise in blood flow or perfusion. These patients are usually observed frequency such as in the intensive care unit. Adaptive Probe Off Detection (APOD) sensitivity is recommended when there is a higher probability of the sensor becoming detached. It is also the recommended mode for areas where patients are not visually monitored continuously. It provides enhanced protection against erroneous pulse rate and SPO_2 readings when the sensor becomes inadvertently detached from a patient due to excessive movement. Maximum sensitivity (MAX) is recommended for patients with weak signals, useful during procedures or when clinician contact is continuous such as high acuity areas.

9.5.6 Response mode (Nellcor)

The Nellcor Oxicable utilizes the OxiMax algorithm which automatically extends the dynamic averaging time for measuring ${\rm SpO_2}$ depending on measurement conditions. There are two response modes available, Normal and Fast. In Normal Mode, the ${\rm SpO_2}$ averaging time is six to seven seconds and in Fast Mode, the ${\rm SpO_2}$ averaging time is approximately three seconds. The Pulse rate averaging time is approximately five seconds, independent of response mode


9.6 Alarm and measurement settings

To change pulse oximetry alarm thresholds and settings:

- 1. Tap ≡ to open the system menu,
- 2. Select Pulse Oximeter Alarms and Settings,
- 3. Tap the desired setting, scrolling if necessary,
- 4. Use the + / buttons to select the required value,
- 5. Tap Confirm to apply the change or Cancel to discard any changes and return to the settings list.

Tap Back twice to return to the Home Screen when you have finished making changes.

All settings are persistent and will retain their previous value when the Airvo 3 is turned on and Same Patient is selected. Selecting New Patient when reviewing the disinfection state applies the default values for its intended clinical environment to all alarm and measurement settings. Refer to the troubleshooting section for troubleshooting SpO₂ measurements and general device alarms.

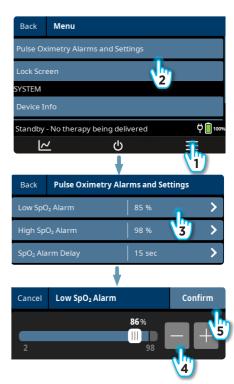


Label	Description	Factory default	Range
Low SpO ₂ Alarm ^{1, 2}	Threshold for SpO ₂ Low alarm	85%	1 - 98%³
High SpO ₂ Alarm ²	Threshold for SpO ₂ High alarm	Off	Off, 2 – 99% ³
SpO ₂ Alarm Delay	Delay before audible Low SpO_2 or High SpO_2 alarm	15 seconds	0, 5, 10, 15 seconds
Averaging Time	Masimo: The length of time to average over Nonin: The number of pulses to average over	8 seconds 8 beats	2-4, 4-6, 8, 10, 12, 14, 16 seconds 4 or 8 beats
Sensitivity Mode	Masimo Only.	APOD	Normal, APOD, Max ⁴
Response Mode	Nellcor Only.	Normal	Normal, Fast

^{1.} The minimum threshold may be set when the device is set up for its intended clinical environment. Refer to the Airvo 3 Technical Manual for details.

- ² The high alarm threshold cannot be set below the low alarm threshold.
- ^{3.} The alarm threshold can be changed in 1% steps.
- 4. Max sensitivity mode does not persist through an Airvo 3 power cycle. Once powered back up the sensitivity setting reverts to the current default setting.

9.7 **Troubleshooting**

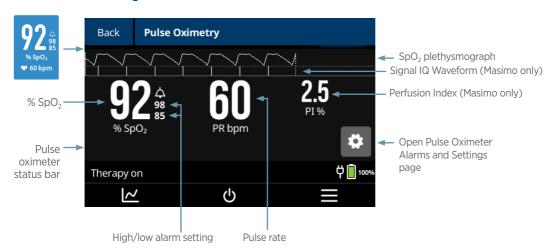

To help ensure successful monitoring of your patient's SpO₂:

- Apply the pulse oximeter sensor to a well-perfused site.
- · Select a measurement site that has unrestricted blood flow.
- · Follow all the instructions supplied with the pulse oximetry sensor to ensure the device is correctly applied.

The pulse oximeter status bar displays the status of the pulse oximeter. Tap the pulse oximeter tile to open the pulse oximetry screen and view the status. Possible status messages and warnings are described below.

Message	Cause/remedy
Low SpO ₂ Signal IQ	Masimo only. The pulse oximeter is indicating low signal confidence in the values displayed due to poor signal strength. The parameters displayed are greyed out while in this state. The patient should be assessed and the sensor should be checked for correct application.
Low Signal Quality	Nonin only. The pulse oximeter is indicating low signal quality. The parameters are displayed in grey while in this state.
	These low signal quality states may be caused by excess motion, low perfusion, a long/blocked light path, or a damaged or incorrectly fitted sensor.
	• Follow the sensor's user instructions to check it is the correct type and that it has been correctly applied to the patient.
	Reduce or eliminate motion at the monitoring site.
	Consider an adhesive sensor.
	 Check that the sensor's emitter and detector are properly aligned, particularly when using an adhesive sensor. Consider a different measurement site.
	Check that blood flow to the measurement site is not restricted.
	 See the pulse oximetry section for physiological conditions that may affect pulse oximetry measurement accuracy and consider an alternative method if indicated.
	Remove excessive fingernail polish or artificial nails.
	Replace the sensor.
Replace Cable Next Patient	Masimo only. The pulse oximetry USB connector cable is defective or has expired and should be replaced after the current patient.
Replace Sensor Next Patient	Masimo only. The pulse oximetry sensor cable is defective or has expired and should be replaced after the current patient.
Sensor Initialising	Masimo only. The pulse oximetry sensor is initialising. If values are not displayed within 30 seconds disconnect and reconnect the sensor. If the problem persists replace the sensor.
Low Perfusion Index	Masimo only. The pulse oximeter is indicating that the perfusion index of the patient is low. Please move the sensor to a better perfused site.

Message	Cause/remedy
Demo mode	Masimo only. The pulse oximeter is indicating that it is running in demonstration mode. If this is unintentional please remove and replace the oximetry equipment.
SpO ₂ Only Mode	Masimo only. The pulse oximeter is indicating that it is running in SpO_2 only mode. No pulse rate is available. Check the sensor placement referring to the directions for use provided with the sensor.
Pulse Search	Masimo and Nellcor only . The pulse oximeter is performing a pulse search. For Nellcor a continuous message indicates a loss-of-pulse while a flashing message indicates searching. If values are not displayed within 30 seconds, disconnect and reconnect the sensor. If the problem persists replace the sensor.
Interference Detected	Masimo and Nellcor only. The pulse oximeter is indicating that interference has been detected. Check that the sensor is correctly applied and if necessary cover the sensor site with an opaque material.
Patient Missing	The pulse oximeter cannot detect a patient. Check that the sensor is properly fitted by following the user instructions supplied with the sensor.
Sensor Disconnected	The pulse oximeter is indicating that there is no sensor currently connected. If there is remove and reconnect. If the problem persists please replace the oximeter accessories.

Nellcor recommends the following actions if there are any issues with their oximetry:

- · Reposition sensor,
- Ensure the sensor is not too tight,
- Try an alternative sensor placement sight,
- · Optically cover the sensor sight,
- · Use an adhesive sensor,
- Use an ear, nasal, or forehead sensor,
- · Use a headband with the forehead sensor,
- · Check the assembly,
- · Remove any nail polish from nail beds,
- · Check for and eliminate external interference,
- · Clean the sensor site.
- Secure the sensor cable.

If pulse oximeter measurements do not correlate with clinical assessment and/or arterial blood gas measurements:

- check the pulse oximeter status, as described above,
- · check the pulse oximeter sensor is fitted correctly, following the user instructions supplied with the sensor,
- · review the pulse oximetry section for conditions that may affect pulse oximetry measurement accuracy and consider an alternative method if indicated, and/or
- · try a different measurement site.

If the Airvo 3 loses mains power, the system will automatically switch over to use the internal battery and pulse oximetry functionality will be maintained including patient settings and trend data.

If mains power is lost and the battery is depleted, pulse oximetry functionality will be lost. It will be restored once power is restored to Airvo 3 maintaining patient settings but trend data will be lost.

Specifications

General	
Dimensions	205 mm x 295 mm x 190 mm
Weight (including battery)	4.45 kg
Supply voltage/current	100-115 VAC, 2.4 A (2.6 A max') 220-240 VAC, 1.1 A (1.3 A max')
Supply frequency	50-60 Hz
USB port sourcing (1 and 2)	5 V, 0.25 A (maximum each port)
Auditory alarm Sound pressure level Audio pause duration	> 40 dBA @ 1 m 120 seconds
Sound level	< 50 dBA @ 1 m
A-weighted sound power level	< 60 dBA
A-weighted sound pressure level	< 50 dBA
Ingress protection	IP22 ²
Expected service life	5 years ³
Operating conditions	
Ambient temperature	18-28 °C
Humidity	10-95% relative humidity (non-condensing)
Ambient pressure	700-1060 hPa

Ambient temperature	18-28 °C
Humidity	10-95% relative humidity (non-condensing)
Ambient pressure	700-1060 hPa
Altitude range	0-3000 m
Mode of operation	Continuous operation
Maximum surface temperature of applied parts ⁴	44 °C
Maximum delivered dew-point temperature of respiratory gas ⁴	43 °C

Storage and transport conditions

Ambient temperature ^{5,6}	-10-50 °C
Humidity (non-condensing)	10-95% relative humidity

Battery (900PT957L)

Chemistry	Lithium Ion (Li-Ion)
Voltage	14.4 VDC
Capacity, Power output	99.4 Wh, 80 W
Battery life ⁷	300 cycles or 2 years from first use (whichever comes first)
Recharge time	6 hours (maximum)
Shelf life	3 years
Operating time	
to 0%8	> 30 minutes
to 20%	
Typical	40 minutes
Worst case ⁹	20 minutes (>30 minutes with flow and supplementary oxygen only)

Supplementary	oxygen
---------------	--------

Oxygen sensor startup time	< 30 s
Oxygen response time	< 60 s
High-pressure oxygen (HPO) inlet port	
Line pressure	280-600 kPa
Maximum flow rate (3 s & 10 s)	100 L/min (STPD10)
% Concentration	93%, > 99%
Low-pressure oxygen (LPO) inlet port	
Line pressure	0-70 kPa
Maximum flow rate	60 L/min (STPD10)
% Concentration	93%, > 99%

Optiflow high flow therapy¹¹

Target humidity range	31-37 °C
Target flow range ¹²	2-70 L/min
Maximum limited pressure ¹³	60 cmH₂O
Maximum operating pressure	< 45 cmH ₂ O
Oxygen concentration	21-100% FiO ₂
Humidity ^{4,7}	
Wall power	> 33 mg/L at 37 °C target humidity, 10-60 L/min target flow ¹⁴
	> 16 mg/L for all other settings
Static temperature stability	±2°C
Warm-up time ¹⁵ (MR290 chamber)	
23 ± 2 °C to 37 °C	< 20 min

- 1. Inrush current may reach 50 A.
- 2. The device is protected against solid objects larger than 12mm (e.g contact with a finger) and vertically dripping water will have no harmful effects when the enclosure is tilted at an angle of up to 15° from its standard position.
- 3. Assumes typical usage pattern. Actual service life may vary.
- 4. In accordance with ISO 80601-2-74. Tested to an accuracy of $\pm\,1\,^{\circ}\text{C}$ or $\pm\,1\,$ mg/L, as appropriate.
- 5. Storage at temperatures above 40 °C for prolonged periods will accelerate battery degradation.
- 6. The device may require up to 24 hours to equilibrate to operating temperature before it is ready for use.
- 7. For humidity performance under battery use, see Appendix 4.
- 8. Worst case battery time from full charged to complete loss of power.
- 9. Worst-case operating time applies to a fully charged battery at 25 °C that has experienced 3 years of storage followed by 300 charge/discharge cycles.
- 10. Flow rate is expressed in STPD (standard temperature and pressure, dry) as per ISO 80601-2-74.
- 11. Values are expressed in body temperature, pressure, saturated (BTPS), in accordance with ISO 80601-2-74, unless otherwise stated.
- 12. Achievable flow range depends on the patient interface selected.
- 13. In accordance with ISO 80601-2-90.
- 14. Applies to use with bypassed airway patient interfaces only.
- 15. Applies when the device is connected to a wall power supply for warm-up.

Range and accuracy of measured parameters

Measurement	Symbol	Displayed Range	Accuracy
Humidity	Temp	31-37 °C	Not specified
Flow rate*	Flow	2-70 L/min	± (1 + 5% of reading) L/min
Oxygen concentration* **	FiO ₂	21-100%	Lower of: ± 4%, or ± (2.5% + 2.5% of reading) - excluding rounding to 21% and 100%, as appropriate - provided "Oxygen concentration" setting is correct
Respiratory rate	RR	4-70 BPM	RMS error of < 3 BPM***
Peripheral blood oxygen saturation	SpO ₂	1-100%	See the specifications sections below.
Pulse rate	PR/♥	Masimo 25-240 beats/min Nellcor 20-300 beats/min Nonin 18-321 beats/min	See the specifications sections below.
Perfusion Index	PI	0.02%-20%	Not specified (Masimo only)

^{*} Test equipment and methods are selected and controlled to ensure the uncertainty coverage is no more than 30% of the disclosed tolerance.

Pulse oximetry specifications (Masimo)

Specifications are tabulated for the Airvo 3 and all compatible sensors unless otherwise stated.

Data update period	< 30 sec
Measurement wavelengths and Output Power	Radiant power with a 50mA pulsed LED is less than 15mW. Masimo's RD SET and LNCS sensors use red and infrared light emitting diodes. The wavelengths for all sensors except TC-I and TF-I sensors are 660 Nanometres (nm), and 905nm for red and infrared respectively. TC-I: 653nm and 880nm for red and infrared respectively. TF-I: 660nm and 880nm for red and infrared respectively. This information is especially useful for clinicians performing photodynamic therapy.

Accuracy (see notes 1-12 below)

Neonates

Saturation (%SpO₂) - During No Motion Conditions

Adults/Pediatrics 70-100% ± 2 digits

0-69% unspecified 70-100% ± 3 digits

Neonates

0-69% unspecified

Saturation (%SpO₂) - During Motion Conditions

Adults/Pediatrics 70-100% ± 3 digits

0-69% unspecified 70-100% ± 3 digits 0-69% unspecified

Pulse Rate (bpm) - During No Motion Conditions

Adults, Pediatric, Neonates

25 to 240 ± 3 digits

Pulse Rate (bpm) - During Motion Conditions

Adults, Pediatric, Neonates

25 to 240 ± 5 digits

^{**} Oxygen measurements are automatically compensated for changes in barometric pressure.

^{***} An RMS accuracy is a statistical calculation of the difference between device measurements and reference measurements. Approximately two-thirds of the device measurements fell within +/- ARMS of the reference measurements in a controlled study.

Resolution

Saturation (%SpO₂) 1% Pulse Rate (bpm) 1

Low Perfusion Performance

Pulse Amplitude + 2 digits % Transmission Saturation (%SpO₂) ± 2 digits ± 3 digits

- 1 The Masimo SET technology with Masimo sensors has been validated for no motion accuracy in human blood studies on healthy adult male and female volunteers with light to dark skin pigmentation in induced hypoxia studies in the range of 70-100% SpO2 against a laboratory CO-Oximeter and ECG monitor. This variation equals ±1standard deviation. Plus or minus one standard deviation encompasses 68% of the population.
- 2 The Masimo SET technology with Masimo sensors has been validated for motion accuracy in human blood studies on healthy adult male and female volunteers with light to dark skin pigmentation in induced hypoxia studies while performing rubbing and tapping motions, at 2 to 4 Hz at an amplitude of 1 to 2 cm and a non-repetitive motion between 1 to 5 Hz at an amplitude of 2 to 3 cm in induced hypoxia studies in the range of 70-100% SpO2 against a laboratory CO-Oximeter and ECG monitor. This variation equals ±1 standard deviation, which encompasses 68% of the population.
- 3. The Masimo SET technology has been validated for low perfusion accuracy in bench top testing against a Biotek Index 2[™] simulator and Masimo's simulator with signal strengths of greater than 0.02% and transmission of greater than 5% for saturations ranging from 70 to 100%. This variation equals ±1 standard deviation. Plus or minus one standard deviation encompasses 68% of the population.
- 4 The Masimo SET Technology with Masimo Neo sensors has been validated for neonatal motion accuracy in human blood studies on healthy adult male and female volunteers with light to dark skin pigmentation in induced hypoxia studies while performing rubbing and tapping motions, at 2 to 4 Hz at an amplitude of 1 to 2 cm and a non-repetitive motion between 1 to 5 Hz at an amplitude of 2 to 3 cm in induced hypoxia studies in the range of 70-100% SpO2 against a laboratory CO-Oximeter and ECG monitor. This variation equals ±1 standard deviation. Plus or minus one standard deviation encompasses 68% of the population, 1% has been added to the results to account for the effects of fetal hemoglobin
- 5 The Masimo SET technology with Masimo sensors has been validated for pulse rate accuracy for the range of 25 -240 bpm in bench top testing against a Biotek Index 2[™] simulator. This variation equals ±1 standard deviation. Plus or minus one standard deviation encompasses 68% of the population.
- 6 See sensor directions for use (DFU) for complete application information. Unless otherwise indicated, reposition reusable sensors at least every 4 hours and adhesive sensors at least every 8 hours
- 7 The TC-I sensor is contraindicated for patients with pierced ears at the measuring site.
- 8 The TF-I sensor must be removed and repositioned to a different monitoring site at least every 2 hours. If extended monitoring is required, use of a single patient adhesive digit sensor
- 9 The TF-I, TC-I, and DBI sensors were not validated under motion conditions
- 10 The Trauma and Newborn sensors are for use only with instruments containing Masimo SET oximetry (Version 4.1.0.1 or higher) or monitors licensed to use specialty sensors.
- 11 Sensor accuracy specified when used with Masimo technology using a Masimo patient cable for LNOP sensors. RD SET sensors, the LNCS sensors, or the M-LNCS sensors, Numbers represent Arms (RMS error compared to the reference). Because pulse oximeter measurements are statistically distributed, only about two-thirds of the measurements can be expected to fall within a range of ± Arms compared to the reference value. Unless otherwise noted, SpO₂ accuracy is specified from 70% to 100%. Pulse Rate accuracy is specified from 25 to 240 bpm.
- 12 Masimo M-LNCS, LNOP, RD, and LNCS sensors, cables, and adapters have the same optical and electrical properties and may differ only in application type (adhesive/non-adhesive/ hook & loop), cable lengths, optical component locations (top or bottom of sensor as aligned with cable), adhesive material type/size, and connector type (LNOP 8 pin modular plug, RD 15 pin modular plug. LNCS 9 pin, cable based, and M-LNCS 15 pin, cable based). All sensor accuracy information and sensor application instructions are provided with the associated sensor directions for use.
- 13 For M-LNCS Blue, LNOP Blue is the predicate, Masimo SET technology with LNOP Blue sensors have been validated for no motion accuracy in human blood studies on neonatal. infant and pediatric patients with congenital cyanotic cardiac lesions in the range of 60%-100% SpO2 against a laboratory co-oximeter. This variation equals plus or minus one standard deviation, which encompasses 68% of the population.
- 14 The presented 510(k) reference is based on the specific FDA clearance for the specific Masimo technology board cleared with the compatible Masimo sensor. The 510(k) reference may vary for the Masimo sensor depending on the pulse oximetry technology (i.e. Masimo SET, Masimo rainbow SET, Philips FAST, Nellcor).

Please refer to the Oxicable Instructions for Use for product specifications.

Pulse oximetry specifications (Nonin)

Specifications are tabulated for the Airvo 3 and all compatible sensors unless otherwise stated.

Nonin:

Data update period	< 30 sec	< 30 sec		
Measurement wavelengths and Output Po		Red: 660 nanometers @ 0.8 mW max. avg.		
	Infrared: 910 nanometers @	Infrared: 910 nanometers @ 1.2 mW max avg. (using Nonin Purelight* sensor)		
SpO ₂ Accuracy (A _{rms} ")	70 to 100%	70 to 100%		
No Motion	Adults/Pediatrics***	Neonates		
Reusable				
8000AX Series:	± 2 digits	N/A		
800XJ Series:	± 3 digits	N/A		
8000SX Series:	± 2 digits	N/A		
8000R:	± 3 digits	N/A		
8000Q2:	± 3 digits	N/A		
Disposable				
6000CX Series:	± 2 digits	± 3 digits		
7000X Series:	± 2 digits	± 3 digits		
Motion				
Reusable				
8000AX Series:	± 2 digits	N/A		
800XJ Series:	± 3 digits	N/A		
8000SX Series:	± 3 digits	N/A		
Low Perfusion****	± 2 digits	± 3 digits		
Pulse Rate Accuracy	Adults/Pediatrics***	Neonates		
No Motion (18 - 300 BPM)				
Reusable				
8000AX Series:	± 3 digits	N/A		
800XJ Series:	± 3 digits	N/A		
8000SX Series:	± 3 digits	N/A		
8000R:	± 3 digits	N/A		
8000Q2:	± 3 digits	N/A		
Disposable				
6000CX Series:	± 3 digits	± 3 digits		
7000X Series:	± 3 digits	± 3 digits		
Motion (40 - 240 BPM)				
Reusable				
8000AX Series:	± 5 digits	N/A		
800XJ Series:	± 5 digits	N/A		
8000SX Series:	± 5 digits	N/A		
Low Perfusion (40 - 240 BPM)****	± 3 digits	± 3 digits		

^{*} This information is especially useful for clinicians performing photodynamic therapy.

Notes:

- SpO₂ accuracy testing is conducted during induced hypoxia studies on healthy, non-smoking, light-to-dark-skinned subjects during motion and no-motion conditions in an independent research laboratory. The measured arterial hemoglobin saturation value (SpO₂) of the sensors is compared to arterial hemoglobin oxygen (SaO₂) value, determined from blood samples with a laboratory co-oximeter. The accuracy of the sensors in comparison to the co-oximeter samples measured over the SpO₂ range of 70 100%. Accuracy data is calculated using the root-mean-squared (Arms value) for all subjects, per ISO 80601-2-61 formerly ISO 9919, Standard Specification for Pulse Oximeters for Accuracy.
- Pulse rate motion testing measures pulse rate accuracy with motion artifact simulation introduced by a pulse oximeter tester. This test determines whether the oximeter meets the criteria of ISO 80601-2-61, formerly ISO 9919, for pulse rate during simulated movement, tremor, and spike motions.
- Low perfusion testing uses an SpO₂ Simulator to provide a simulated pulse rate, with adjustable amplitude settings at various SpO₂ levels. The module must maintain accuracy in accordance with ISO 80601-2-61, formerly ISO 9919, pulse rate and SpO₂ at the lowest obtainable pulse amplitude (0.3% modulation).

^{**} $\pm\,1\,A^{\mbox{\tiny rms}}$ represents approximately 68% of measurements.

^{***} Includes Infant patients

^{****} Does not apply to those sensors listed as N/A under the neonate column, 8000R and 8000Q2

- The Nonin Xpod has been validated for pulse rate accuracy from 18-300 bpm with no motion and from 40-240 bpm with motion. Testing was carried out using a Datrend Oxitest Plus 7 simulator
- Low perfusion testing uses an SpO₂ Simulator to provide a simulated pulse rate, with adjustable amplitude settings at various SpO₂ levels. The module must maintain accuracy in accordance with ISO 80601-2-61, formerly ISO 9919, pulse rate and SpO₂ at the lowest obtainable pulse amplitude (0.3% modulation).

Standards compliance

Designed to conform to the following standards:

IEC 60601-1:2005+AMD1:2012 +AMD2:2020 IEC 60601-1-2:2014+AMD1:2020



Medical — cardio, vascular and pulmonary equipment as to electrical shock, fire and mechanical hazards only in accordance with AAMI ES60601-1 (2005) + AMD 1 (2012), CSA CAN/CSA-C22.2 NO. 60601-1:14, IEC 60601-1-6:2010, AMD1:2013, IEC 60601-1-8: 2006 + Am.1: 2012, ISO 80601-2- 61:2017, COR1:2018, ISO 80601-2-74:2017

ANSI/AAMI ES 60601-1:2005 and A1:2012 and A2:2021

CAN/CSA-C22.2 NO.60601-1:14+A2:2022 (R2022)

IEC 60601-1-6:2010+AMD1:2013+AMD2:2020

IEC 60601-1-8:2006+AMD1:2012+AMD2:2020

IEC 60601-1-10:2007+AMD1:2013+AMD2:2020

ISO 80601-2-61:2017

ISO 80601-2-74:2021

Do not place any part of the device or accessories within 30 cm of any portable mobile radio frequency communication equipment. The Airvo 3 complies with the electromagnetic compatibility requirements of IEC 60601-1-2. In certain circumstances the Airvo 3 may affect or be affected by nearby equipment because of electromagnetic interference. Excessive electromagnetic interference may affect the therapy delivered by the device. If this should happen, try moving the Airvo 3 or the unit causing interference, or consult your healthcare provider.

FCC compliance

This device has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This device generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this device does cause harmful interference to radio or television reception, which can be determined by turning the device off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reposition or relocate the receiving antenna.
- Increase the separation between the device and receiver.
- Connect the device into an outlet on a circuit different from that to which the receiver is connected.
- Consult your healthcare provider or your Fisher & Paykel Healthcare representative for help.

Accessory equipment connected to the any port of the Airvo 3 must be certified to IEC 60601-1-1 or IEC 60950-1. All configurations shall comply with the system standard IEC 60601-1-1. Anyone who connects additional equipment to the signal input part or signal output part configures a medical system and is therefore responsible for ensuring that the system complies with the requirements of the system standard IEC 60601-1-1. If in doubt, consult your technical services department or your local Fisher & Paykel Healthcare representative.

Certain elements of the software included with product are supplied under the license terms of third parties, including elements of the software that are subject to certain open source software licenses. Where required by the terms of these licenses, Fisher & Paykel Healthcare Limited provides notices regarding such software elements on its website. Please visit www.fphcare.com/airvo3/ third-party-licenses to view these notices. Note that the notices that apply may be updated as the software included in the product is updated. The F&P Airvo 3 is in compliance with Directive 2014/53/EU. The full text of the EU declaration of conformity is available at the following internet address: www.fphcare.com/certifications.

Device disposal instructions



This device contains electronic components and a lithium-ion battery. Regulations in your country may require them to be collected for waste recovery and recycling to reduce the environmental impact. Please dispose of this device in accordance with local regulations.


Disposal of accessories, spare parts and packaging



Dispose of accessories, spare parts and packaging according to local guidelines. Place the breathing tube and water chamber in a waste bag at the end of use and discard with normal waste. Hospitals should discard according to their standard method for disposing of contaminated product.

Glossary

Symbols

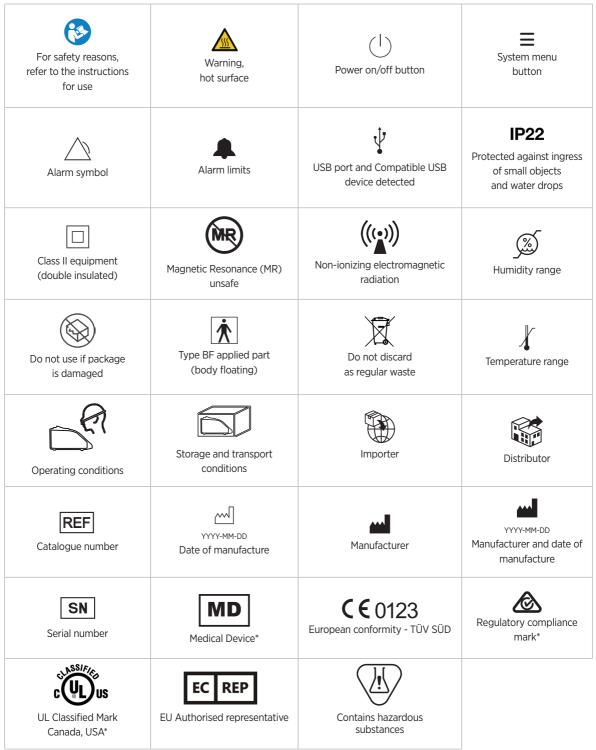

^{*}symbol seen on select models

Appendix 1. Patient consumables

The patient interfaces and accessories shown in the tables below are approved for use with the Airvo 3. Carefully read the user instructions, including all warnings and cautions, supplied with each device before use.

Some accessories may not be available in certain countries. Contact your Fisher & Paykel representative for the latest information on patient interfaces available for the Airvo 3. All patient interfaces are Type BF applied parts.

Optiflow high flow therapy

Description	Part number	Size	Pack size
Optiflow+ nasal interface	OPT942	Small	20
	OPT944	Medium	20
	OPT946	Large	20
Optiflow+ Duet interface	OPT962	Small	20
	OPT964	Medium	20
	OPT966	Large	20
Optiflow 3S nasal interface	OPT1042	Small	20
	OPT1044	Medium	20
	OPT1046	Large	20
Optiflow Junior 2 nasal interface*	OJR414 (WJR112)	М	20 (20)
	OJR416 (WJR112)	L	20 (20)
	OJR418 (WJR112)	XL	20 (20)
Optiflow Junior 2+ nasal interface*	OJR520 (WJR114)	XXL	10 (10)
Optiflow Junior 2 WigglewiNG	WJR212	M, L, XL	20
	WJR214	XXL	10
Optiflow+ tracheostomy interface	OPT970	15 mm	20
Optiflow+ mask interface adapter**	OPT980	22 mm mask interface adapter	20
AirSpiral tube and chamber kit	900PT561	_	10
AirvoNeb tube and chamber kit	900PT562	_	10

^{*} Wigglepads part numbers are shown in parentheses.

^{**} The mask adapter interface is designed for vented masks only. Do not use sealed masks with Optiflow high flow therapy.

Appendix 2. Parts and accessories

Some accessories may not be available in certain countries. Please contact your local Fisher & Paykel Healthcare representative for more information.

Accessories

Description	Part number
Mobile pole stand	900PT421
Mobile pole stand handle	900PT445
Mobile pole stand clamp	900PT428
Oxygen-bottle holder	900PT427, 900PT427L
Storage basket	900PT426
Storage cover	900PT603
HPO Dual-Input Manifold (DISS, NIST, SIS)	900PT460D, 900PT460N, 900PT460S
HPO adapter (DISS to NIST)	900PT462DN
Airvo 3 data port adapter*	900PT473
Airvo 3 USB service cable	900PT474
Fisher & Paykel Healthcare Device Manager	900PT475
Disinfection kit**	900PT600

^{*} The data port adapter allows for data to be transferred from the Airvo 3 to patient monitoring and hospital computer systems. Integration is required to enable functionality.

^{**}A disinfection kit is required when using the built-in disinfection mode to disinfect the outlet elbow. It is not required for hospitals using a washer-disinfector to clean and disinfect the outlet elbow.



△ Warnings

Equipment connected to Airvo 3 via the Data Port Adaptor (900PT473) must be certified according to IEC 60950-1 or IEC 60601-1. All combinations of equipment must be in compliance with IEC 60601-1 requirements for medical electrical systems. Any person who connects additional equipment has now configured a medical system and is therefore responsible for ensuring that the system complies with the requirements of IEC 60601-1. Consult a technical specialist in your hospital for more information.

Using accessories other than those specified may result in increased electromagnetic emissions or decreased electromagnetic immunity of the Airvo 3.

All data transferred from Airvo 3 is intended for information only and must not be used as the sole basis for diagnostic or therapeutic decisions.

Spare parts

Part number
900PT602
900PT603
900PT930
900PT933
900PT957L

Appendix 3. Pulse oximetry accessories

The pulse oximetry accessories listed below are compatible with the Airvo 3. Carefully read the user instructions, including all warnings and cautions, supplied with each device before use. Not all accessories are available in all markets, and some accessories may not be available from Fisher & Paykel Healthcare.

Masimo:

Part numbers of compatible Masimo pulse oximetry USB connector cable, adapters, and extension cables

Description	Masimo part number (cable length)
uSpO₂ Masimo SET Oximetry Cable, USB	3412 (1.8m)
RD to LNC Adapter Cable	4089 (0.9m)
RD to LNC Adapter Cable	4105 (0.45m)
LNC-4-Ext	2021 (1.2m)

Part numbers of compatible Masimo pulse oximetry sensor cables and sensor consumables

Sensor description	Masimo part number (cable length) (other information)
RD SET [™] DCI Series Adult Reusable Finger Clip Sensors	4050 (0.9m)
RD SET [™] DCI-P Series Pediatric Reusable Finger Clip Sensors	4051 (0.9m)
RD SET [™] TC-I Reusable Tip Clip Sensor	4053 (0.9m)
RD SET [™] YI SpO ₂ Multisite Reusable Sensor	4054 (0.9m)
$RD SET^{M} TF-I SpO_{2}$ Reusable Transflectance Forehead Sensor	4055 (0.9m)
RD SET [™] DB-I Reusable Soft Sensors	4052 (0.9m)
RD SET [™] Series Adt SpO ₂ Disposable Sensors	4000 (0.45m) (20 pack)
RD SET [™] Series Pdt SpO ₂ Disposable Sensors	4001 (0.45m) (20 pack)
RD SET [™] Series Inf SpO ₂ Disposable Sensors	4002 (0.45m) (20 pack)
RD SET [™] Series Neo SpO ₂ Disposable Sensors	4003 (0.45m) (20 pack)
RD SET [™] Series Neo Pt SpO ₂ Disposable Sensors	4004 (0.45m) (20 pack)
RD SET Series Neo Pt SpO ₂ Disposable Sensors (Non-Adhesive)	4005 (0.45m) (20 pack)
RD SET [™] Speciality Sensor Series Adult Trauma	4011 (10 pack)
RD SET [™] Specialty Sensor Series Newborn Neonatal	4013 (10 pack)
RD SET [™] Specialty Sensor Series Newborn, Infant, Pediatric	4012 (10 pack)
RD SET [™] Blue Disposible Sensor	4014 (10 pack)
RD SET [™] Ear Sensor	4015 (0.9m) (10 pack)
$RD SET^{TM} TFA-1 SpO_2$ Disposable Transflectance Forehead Sensor	4016 (0.9m)
LNCS®DCI ADT Reusable Sensor	1863 (0.9m)
LNCS®DCIP Reusable Sensor	1864 (0.9m)
LNCS®TC-I Reusable Tip Clip Sensor	1895 (0.9m)

Masimo®, Adaptive Probe Off Detection®, APOD®, LNCS®, SET®, Signal Extraction Technology®, Signal I.Q.®, uSpO,®, X-Cal®, RD SET™ are trademarks of Masimo Corporation.

Masimo:

Part numbers of compatible Masimo pulse oximetry sensor cables and sensor consumables

Sensor description	Masimo part number (cable length)
LNCS®YI SpO ₂ Multisite Reusable Sensor	2258 (0.9m)
LNCS®TF-I® Adult SpO₂ Reusable Transflectance Sensor	1896 (0.9m)
LNCS® DB-I Series Reusable Soft Sensors	2653 (0.9m)
LNCS® Adtx, Adult Adhesive Sensor	1859 (0.45m) (20 pack)
LNCS® Adtx-3, Adult Adhesive Sensor	2317 (0.9m) (20 pack)
LNCS® Pdtx, Pediatric Adhesive Sensor	1860 (0.45m) (20 pack)
LNCS® Pdtx-3, Pediatric Adhesive Sensor	2318 (0.9m) (20 pack)
LNCS [®] Inf, Infant Adhesive Sensor	2328 (0.45m) (20 pack)
LNCS® Inf-3, Infant Adhesive Sensor	2319 (0.9m) (20 pack)
LNCS [®] Inf-L, Infant Adhesive Sensor	1861 (0.9m) (20 pack)
LNCS [®] Neo, Neonate Adhesive Sensor	2329 (0.45m) (20 pack)
LNCS® Neo-3, Neonate Adhesive Sensor	2320 (0.9m) (20 pack)
LNCS® Neo-L, Neonate Adhesive Sensor	1862 (0.9m) (20 pack)
LNCS® NeoPt, Sensitive Skin Neonate Adehesive Sensor	2330 (0.45m) (20 pack)
LNCS® NeoPt-3, Sensitive Skin Neonate Adhesive Sensor	2321 (0.9m) (20 pack)
LNCS® NeoPT-L, Sensitive Skin Neonate Adhesive Sensor	1901 (0.9m) (20 pack)
LNCS® NeoPt-500, Neonate Non-Adhesive Sensor	2331 (0.45m) (20 pack)
LNCS® Trauma Adult Adhesive Sensor	2411 (0.9m) (20 pack)
LNCS® Specialty Sensor Series Newborn neonatal	2412 (0.9m) (20 pack)
LNCS® Specialty Sensor Series Newborn, Infant, Pediatric	2413 (0.9m) (20 pack)
LNCS [®] E1 Ear Sensor	2918 (0.9m) (10 pack)
${\rm LNCS}^{\circledast}{\rm TFA-1}{\rm SpO_2}{\rm Disposable}{\rm Transflectance}{\rm Forehead}{\rm Sensor}$	3858 (0.9m) (10 pack)

 $Masimo^*, Adaptive\ Probe\ Off\ Detection^*, APOD^*, LNCS^*, SET^*, Signal\ Extraction\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masimo\ Technology\ ^*, Signal\ I.Q.^*, uSpO_2^*, X-Cal^*, RD\ SET^{\text{Int}}\ are\ trademarks\ of\ Masi$ Corporation.

Nellcor:

Adaptors and extension cables

Description	Part number
Pulse Oximetry Connection Converter 1	900PT476 (0.3m)
Medtronic/Nellcor Oxicable	PMC10N-SF (2.8m)

Part numbers of compatible Nellcor pulse oximetry sensor consumables

Sensor description	Nellcor part number (cable length) (other information)
Nellcor SpO₂ Forehead Sensor	MAXFAST (0.75m) (24 pack)
Nellcor SpO ₂ Nonadhesive Sensor	SC-A/SC-NEO/SC-PR (0.9m) (24 pack)
Nellcor Flexible SpO₂ Sensor	FLEXMAX/FLEXMAX-P (0.9m)
Nellcor SpO ₂ Adhesive Sensors	MAXA/MAXAL/MAXN/MAXI/MAXP (0.9m) (24 pack)
Nellcor SpO₂ Adhesive Sensors Nasal	MAXR (0.45m) (24 pack)
Nellcor Reusable SpO₂ Sensors	DS100A (1 pack), OXI-A, OXI-N, OXI-P, OXI-I (24 pack) (0.9m)
Nellcor Reusable Multisite SpO ₂ Sensors	D-YS, D-YSE, D-YSPD (0.9m), PDSLV (replacement sleeves, 12 pack)
Nellcor Single-Patient Use Sensor Wraps	POSEY (for OXI-A/N/P/I, D-YS) (12 pack)
Nellcor Single-Patient Use Adhesive Sensor Wraps	ADH-A/N (for OXI-A/N, D-YS), ADH-P/I (for OXI-P/I, D-YS) (100 pack)
Nellcor Single-Patient Use Foam Sensor Wraps	FOAM A/N (for OXI-A/N, D-YS), FOAM P/I (for OXI-P/I, D-YS) (100 pack)

 $Nellcor^{{\scriptscriptstyle TM}}, OxiMax^{{\scriptscriptstyle TM}}, OxySoft^{{\scriptscriptstyle TM}}, Oxymax^{{\scriptscriptstyle TM}}, Satseconds^{{\scriptscriptstyle TM}}, Medtronic^{{\scriptscriptstyle TM}} \ are \ trademarks \ of \ Medtronic \ PLC.$

Nonin:

Part numbers of compatible Nonin pulse oximetry USB connector cables

Description	Nonin part number (cable length)
Nonin Xpod 3012HR USB Connector Cable	114403-001 (1m)
Xpod® 3012 LP with USB Connector	6703-001 (1m)

Part numbers of compatible Nonin pulse oximetry sensor cables and sensor consumables

Sensor description	Nonin part number (cable length) (other information)
8000SS reusable soft sensors, small	6837-000 (1m), 6837-300 (3m)
8000SM reusable soft sensors, medium	6836-000 (1m), 6836-300 (3m)
8000SL reusable soft sensors, large	6835-000 (1m), 6835-300 (3m)
8000AA adult reusable finger clip sensors	3278-001 (1m), 3278-006 (2m, 6.6m), 3278-003 (3m)
8000AP pediatric reusable finger clip sensors	2360-000 (1m), 2360-003 (3m)
8000Q2 ear clip sensor	6455-000 (1m)
8000R reflectance sensor	0487-000 (1m)
8000J adult semi-reusable Flex Sensor	0741-000 (1m), 2353-002 (3m) (includes x25 8000JFW FlexiWraps*)
8008J infant semi-reusable Flex Sensor	0740-000 (1m) (includes x25 8008JFW FlexiWraps)
8001J neonatal semi-reusable Flex Sensor	0739-000 (1m) (includes x25 8001JFW FlexiWraps)
6000CA adult cloth disposable sensors	7426-001 (lm) (24 pack)
6000CP pediatric cloth disposable sensors	7426-002 (1m) (24 pack)
6000Cl infant cloth disposable sensors	7426-003 (1m) (24 pack)
6000CN neonatal cloth disposable sensors	7426-004 (1m) (24 pack)
7000A adult Flexi-Form* III disposable sensors	7427-001 (1m) (24 pack)
7000P pediatric Flexi-Form III disposable sensors	7427-002 (1m) (24 pack)
7000I infant Flexi-Form III disposable sensors	7427-003 (1m) (24 pack)
7000N neonatal Flexi-Form III disposable sensors	7427-004 (1m) (24 pack)
8000JFW adult FlexiWraps	4097-000, (25 pack), for use with 8000J
8008JFW infant FlexiWraps	4774-000, (25 pack), for use with 8008J
8001JFW neonatal FlexiWraps	4777-000, (25 pack), for use with 8001J
8000H reflectance sensor holder pack	0616-000, (10 caps & 20 adhesive stickers) for use with 8000R
Sensor Clip for LP Xpod External Pulse Oximeter	7504-001


Nonin™, Xpod®, PureLight®, PureSAT®, FlexiWraps®, Flexi-Form® are trademarks of Nonin Medical Inc.

Appendix 4. Humidification behavior during battery operation

The Airvo 3 reduces the energy used to humidify breathing gases when not powered from a wall power supply, to conserve battery power. In all cases, the Airvo 3 continues supplying supplementary oxygen and breathing gases until the battery is depleted.

For Optiflow high flow therapy, active humidification of the breathing gases is reduced during battery operation. If the Critically Low Battery alarm is raised, active humidification is stopped to conserve battery power.

Connect the Airvo 3 to a wall power supply before the battery is empty to automatically resume normal therapy. If the Airvo 3 battery is depleted, the device stops supplying supplementary oxygen and breathing gases, powers down and produces the Power Out alarm. To resume therapy after the device has powered down, connect the Airvo 3 to a wall power supply.

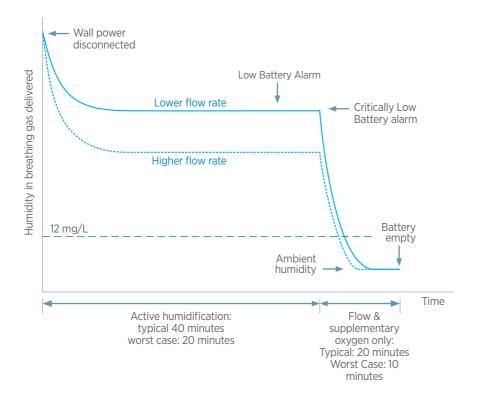

The Airvo 3 delivers reduced humidity in the breathing gas during Optiflow high flow therapy until the battery is nearly depleted, where humidity is turned off to maintain the delivery of flow and oxygen.

Masimo End User License Agreement



END-USER LICENSE AGREEMENT

THIS DOCUMENT IS A LEGAL AGREEMENT BETWEEN YOU ("PURCHASER") AND FPH. IF YOU DO NOT AGREE TO THE TERMS OF THIS AGREEMENT, PROMPTLY RETURN THE ENTIRE PACKAGE, INCLUDING ALL ACCESSORIES, IN THEIR ORIGINAL PACKAGE, WITH YOUR SALES RECEIPT TO FPH FOR A FULL REFUND.

- a. <u>Grant of License.</u> In consideration of payment of the license fee, which is part of the price paid for this product. FPH grants to Purchase a nonexclusive, nontransferable license, without right to sub-license, to use the copy of the incorporated software/firmware, and documentation in connection with Purchaser's use of Masimo products for their labeled purpose. FPH reserves all rights not expressly granted to purchaser.
- b. Ownership of Software/Firmware. Title to, ownership of, and all rights and interests in, any Masimo software and/or firmware and the documentation, and all copies thereof, remain at all times vested in Masimo Corporation, licensor to FPH, and they do not pass to purchaser.
- c. <u>Assignment.</u> Purchaser shall not assign or transfer this License, in whole or in part, by operation of law or otherwise, without FPH's prior written consent; any attempt without such consent, to assign any rights, duties or obligations arising hereunder shall be void.
- d. <u>Copy Restrictions</u>. The software/firmware, mask works, circuit board layouts, and accompanying written materials are copyrighted. Unauthorized copying of the software, including software that has been modified. Unauthorized copying of the software, including software that has been modified, merged, or included with other software, or other written materials is expressly forbidden. You may be held legally responsible for any copyright infringement that is cause or incurred by your failure to abide by the terms of this license. Nothing in this license provides any rights beyond those provided by 17 U.S.C 117.
- E. <u>Use Restriction.</u> As the Purchaser, you may physically transfer the products from one location to the another provided that the software/firmware is not copied. You may not electronically transfer the software/firmware from the products to any other device. You may not disclose, publish, translate, release distributed copies of, modify, adapt, translate, reverse engineer, decompile, disassemble, or create derivative works based on the Masimo product, the software/firmware, or the written materials without the prior written consent of Masimo. Masimo sensors that are designated for single use are licensed under Masimo patents for use on a single patient only, and are not sold. Possession of a Masimo device does not convey any express or implied license to use the device with unauthorized sensors or cables that would, alone, or in combination with this device, fall within the scope of one or more of the patents relating to the device. There is no license, implied or otherwise, that would allow use of single use Masimo Sensors beyond their intended single use. After use of single use Masimo sensors, there is no further license granted by Masimo to use the sensors and they must be discarded.
- f. Non-authorized Accessories. Masimo technology is designed to operate together with Masimo devices, cables, sensors, and accessories as an integrated system. When any component of the system is compromised, erroneous measurements can occur. Accordingly, the use of unauthorized cables, sensors, or accessories, such as third-party reprocessed or copycat sensors, can yield unreliable results when used with a Masimo device. The performance of Masimo technology is not validated when used with any unauthorized cable, sensor, or accessory.
- g. <u>Transfer restrictions</u>. The software/firmware is licensed to the Purchaser and may not be transferred to anyone, except other end-users, without the prior written consent of FPH. In no event may you transfer, assign, rent, lease, sell, or otherwise dispose of the software/firmware or the products on a temporary basis.
- h. <u>Beneficiary.</u> Masimo Corporation is a Beneficiary of this Agreement and has the right to enforce its provisions.
- I. <u>U.S Government Rights</u>: If you are acquiring software (including the related documentation) on behalf of any part of the United States Government, the following provisions apply: the software is deemed to be "commercial software" and "commercial computer software documentation", respectively pursuant to DFAR section 227.7202 FAR 12.212 as applicable. Any use, modification, reproduction, release, performance, display or disclosure of the software (including the related documentation) by the U.S Government or any of its agencies shall be governed solely by the terms of this agreement.





Fisher & Paykel Healthcare Ltd, 15 Maurice Paykel Place, East Tamaki, Auckland 2013, PO Box 14 348 Panmure, Auckland 1741, New Zealand Tel: +64 9 574 0100 Email: info@fphcare.co.nz Web: www.fphcare.com



Australia (AU) (Sponsor) Fisher & Paykel Healthcare Pty Ltd, 19-31 King Street, Nunawading, Melbourne, Victoria 3131. Tel: +61 3 9871 4900 Brazil (BR) Fisher & Paykel do Brasil, Rua Sampaio Viana, 277 cj 21, Paraíso, 04004-000, São Paulo - SP, Brazil Tel: +55 11 2548 7002 China (CN) 代理人售后服务机构:费雪派克医疗保健 (广州) 有限公司,广州高新技术产业开发区科学城科丰路31号G12栋301号 电话: +88 20 32053486 Colombia (CO) Tel: +57 3142852934 France (FR) 医 Pisher & Paykel Healthcare SAS, 10 Av. du Québec, Bât F5, BP 512, Villebon-sur-Yvette, 91946 Courtaboeuf Cedex, France Tel: +33 1 6446 5201 Email: c.s@fphcare.fr Germany (DE) Fisher & Paykel Healthcare GmbH, Wiesenstrasse 49, 73614 Schorndorf, Germany Tel: +49 7181 98599 0 Hong Kong (HK) Tel: +852 2116 0032 India (IN) Tel: +91 80 2309 6400 Japan (JP) Tel: +81 3 5117 7110 Fax: +81 3 5117 7115 Korea (KR) Tel: +82 2 6205 6900 Mexico (MX) Tel: +52 55 9130 1626 Poland (PL) Fisher & Paykel Healthcare Poland Sp. z o.o., Pl. Andersa 7, 61-894 Poznań, Poland Tel: +48 664 846 464 Russia (RU) Tel: +7 495 782 21 50 Sweden (SE) Fisher & Paykel Healthcare AB, Svetsarvägen 15, 2tr, 17141 Solna, Sweden Tel: +46 8 564 76 680 Switzerland (CH) CH REP Fisher & Paykel Healthcare GmbH, Sāntisstrasse 2, 9501 Wil / SG, Switzerland Tel: 0800 83 47 63 Taiwan (TW) Tel: +886 2 8751 7739 Turkey (TR) Ithalatcı Firma: Fisher Paykel Sağlık Ürünleri Ticaret Limited Şirketi, İletişim Bilgileri: Ostim Mahallesi 1249. Cadde No:6, Yenimahalle, Ankara, Türkiye 06374, Tel: +90 312 354 34 12 UK (GB) W REP Fisher & Paykel Healthcare Ltd, Unit 16, Cordwallis Park, Clivemont Road, Maidenhead, Berkshire SL6 7BU, UK Tel: 0800 132 189 USA (US)/Canada (CA) Tel: 1800 446 3908 or +1 949 453 4000



Austria (AT) Tel: 0800 29 31 23 Benelux (BE NL LU) Tel: +31 40 216 3555 Denmark (DK) Tel: +45 70 26 37 70 Finland (FI) Tel: +358 9 251 66 123 Ireland (IE) Tel: 1800 409 011 Italy (IT) Tel: +39 06 7839 2939 Norway (NO) Tel: +47 21 60 13 53 Spain (ES) Tel: +34 902 013 346

For more information, please contact your local Fisher & Paykel Healthcare representative.



