



FITTING GUIDE

FITTING*

1 Select cannula size

Select appropriate cannula size; A clear gap must be visible around each prong. The sizing chart on the following page should only be used as a guide.

2 Prepare skin

Prepare the patient's skin according to hospital protocol.

3 Connect to gas source

Connect the system to the gas source and ensure there is gas flow through the prongs.

4 Remove the first F&P Wigglepad™ 2 tabs

Remove the first backing tabs from the F&P Wigglepads 2 and avoid touching the adhesive.

5 Insert cannula

Insert the cannula into the nares. Ensure the cannula bridge rests close to the nose without touching the septum. DO NOT stretch the cannula during application. Stick the F&P Wigglepads 2 to the patient's cheeks.

6 Secure cannula

Remove the second backing tabs and stick the F&P Wigglepads 2 onto the cheeks.


1 SELECT CANNULA SIZE

SIZE RANGE

XXL
OJR520



ENSURE GAP AROUND PRONGS*



4

First backing tab



Second backing tab

5



6

Second backing tabs




* IMPORTANT: Always refer to the user instructions supplied with the product for full set up instructions, warnings, cautions and contraindications.



REMOVE CANNULA

1 Place fingertip

Place fingertip on the outside edge of the F&P Wigglepads 2 and gently peel the cannula away from the Wigglepads 2. Starting from the outside, peel towards the nose.

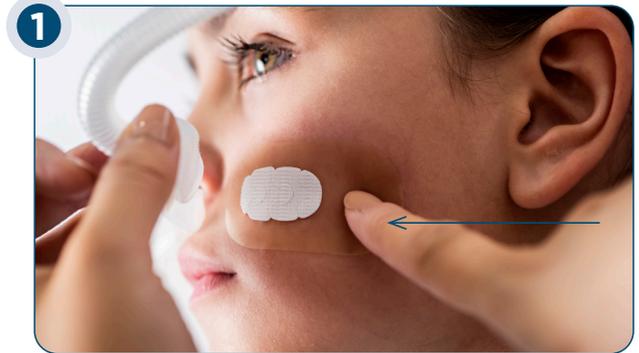

F&P WIGGLEPADS 2 REMOVAL & REPLACEMENT

1 Lift the edge

Lift the edge of the F&P Wigglepads 2. Use a damp cloth to wipe the patient's skin and the underside of the Wigglepads 2 while gently peeling away from the patient's face.



2 Adhere

Adhere the replacement F&P Wigglepads 2 to the cannula, remove the first backing tabs and stick the Wigglepads 2 onto the patient's cheeks.



3 Remove

Remove the second backing tabs and stick onto the patient's cheeks.

SIZING INFORMATION

1. Prongs must not create a seal in the nares. A clear gap must be visible around each prong.
2. Patient weight should only be used as a guide.

	WEIGHT GUIDE (KG)					SPARES
	0	8	12.5	20	30	
OJR520 XXL 						
						F&P Wigglepads™ 2 WJR114 

Expected to fit patient
 May fit patient

Optiflow, Wigglepads and Dolphin are trademarks of Fisher & Paykel Healthcare Limited. For patent information, see www.fphcare.com/ip

615570 REV A 2020-01 © 2019 Fisher & Paykel Healthcare Ltd